

(19)

Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11) EP 0 958 495 B1

(12)

## EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention  
of the grant of the patent:  
**13.11.2002 Bulletin 2002/46**

(51) Int Cl. 7: **G01N 27/327, C12Q 1/00**

(21) Application number: **98906328.4**

(86) International application number:  
**PCT/US98/02652**

(22) Date of filing: **06.02.1998**

(87) International publication number:  
**WO 98/035225 (13.08.1998 Gazette 1998/32)**

### (54) SMALL VOLUME IN VITRO ANALYTE SENSOR

KLEINVOLUMIGER SENSOR ZUR IN-VITRO BESTIMMUNG

DETECTEUR D'UN FAIBLE VOLUME D'ANALYSTE IN VITRO

(84) Designated Contracting States:  
**AT BE CH DE DK ES FI FR GB GR IE IT LI LU MC  
NL PT SE**

• **TOMASCO, Michael, F.  
Cupertino, CA 95014 (US)**

(30) Priority: **06.02.1997 US 795767**

(74) Representative: **Andrae, Steffen, Dr. et al  
Andrae Flach Haug  
Balanstrasse 55  
81541 München (DE)**

(43) Date of publication of application:  
**24.11.1999 Bulletin 1999/47**

(56) References cited:  
**EP-A- 0 255 291 EP-A- 0 286 084  
WO-A-95/02817 WO-A-95/13534  
US-A- 5 120 420 US-A- 5 130 009  
US-A- 5 437 999**

(73) Proprietor: **Therasense, Inc.  
Alameda, CA 94502 (US)**

• **C. W. ANDERSON ET AL: "A small volume  
thin-layer spectroelectrochemical cell for the  
study of biological components." ANALYTICAL  
BIOCHEMISTRY, vol. 93, no. 2, 1979, pages  
366-372, XP002068329**

(72) Inventors:  
• **HELLER, Adam  
Austin, TX 78731 (US)**  
• **FELDMAN, Benjamin, J.  
Oakland, CA 94618 (US)**  
• **SAY, James  
Alameda, CA 94501 (US)**  
• **VREEKE, Mark, S.  
Alameda, CA 94501 (US)**

EP 0 958 495 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description**

**Field of the Invention**

5 [0001] This invention relates to analytical sensors for the detection of bioanalytes in a small volume sample.

**Background of the Invention**

10 [0002] Analytical sensors are useful in chemistry and medicine to determine the presence and concentration of a biological analyte. Such sensors are needed, for example, to monitor glucose in diabetic patients and lactate during critical care events. For example, U.S. Pat. No. 5,120,420 discloses a biosensor having an insulating base board having formed thereon, in sequence, leads an electrode system mainly made of carbon, an insulating layer and a reaction layer composed of an enzyme and an electron acceptor, and being provided thereon with a space defined by a spacer and a cover.

15 [0003] Currently available technology measures bioanalytes in relatively large sample volumes, e.g., generally requiring 3 microliters or more of blood or other biological fluid. These fluid samples are obtained from a patient, for example, using a needle and syringe, or by lancing a portion of the skin such as the fingertip and "milking" the area to obtain a useful sample volume. These procedures are inconvenient for the patient, and often painful, particularly when frequent samples are required. Less painful methods for obtaining a sample are known such as lancing the arm or 20 thigh, which have a lower nerve ending density. However, lancing the body in the preferred regions typically produces submicroliter samples of blood, because these regions are not heavily supplied with near-surface capillary vessels.

[0004] It would therefore be desirable and very useful to develop a relatively painless, easy to use blood analyte sensor, capable of performing an accurate and sensitive analysis of the concentration of analytes in a small volume of sample.

25

**Summary of the Invention**

30 [0005] The sensors of the present invention provide a method for the detection and quantification of an analyte in submicroliter samples. In general, the invention includes a method and sensor for analysis of an analyte in a small volume of sample, preferably by coulometry, as defined in the claims.

**Brief Description of the Drawings**

35 [0006] Referring now to the drawings, wherein like reference numerals and letters indicate corresponding structure throughout the several views:

Figure 1 is a schematic view of a first embodiment of an electrochemical sensor in accordance with the principles of the present invention having a working electrode and a counter electrode facing each other;

40 Figure 2 is a schematic view of a second embodiment of an electrochemical sensor in accordance with the principles of the present invention having a working electrode and a counter electrode in a coplanar configuration;

Figure 3 is a schematic view of a third embodiment of an electrochemical sensor in accordance with the principles of the present invention having a working electrode and a counter electrode facing each other and having an extended sample chamber;

45 Figure 4 is a not-to-scale side-sectional drawing of a portion of the sensor of Figures 1 or 3 showing the relative positions of the redox mediator, the sample chamber, and the electrodes;

Figure 5 is a top view of an embodiment of a multiple electrode sensor in accordance with the principles of the present invention;

Figure 6 is a perspective view of an embodiment of an analyte measurement device in accordance with the principles of the present invention having a sample acquisition means and the sensor of Figure 4;

50 Figure 7 is a graph of the charge required to electrooxidize a known quantity of glucose in an electrolyte buffered solution (filled circles) or serum solution (open circles) using the sensor of Figure 1 with glucose oxidase as the second electron transfer agent;

Figure 8 is a graph of the average glucose concentrations for the data of Figure 7 (buffered solutions only) with calibration curves calculated to fit the averages; a linear calibration curve was calculated for the 10-20 mM concentrations and a second order polynomial calibration curve was calculated for the 0-10 mM concentrations;

55 Figure 9 is a Clarke-type clinical grid analyzing the clinical relevance of the glucose measurements of Figure 7;

Figure 10 is a graph of the charge required to electrooxidize a known quantity of glucose in an electrolyte buffered solution using the sensor of Figure 1 with glucose dehydrogenase as the second electron transfer agent;

Figures 11A, 11B, and 11C are top views of three embodiments of an electrochemical sensor of the present invention;

Figures 12A and 12B are cross-sectional views of another embodiment of an electrochemical sensor of the present invention formed using a recess of a base material;

Figures 13A and 13B are cross-sectional views of yet another embodiment of an electrochemical sensor or the present invention formed in a recess of a base material; and

Figures 14A and 14B are cross-sectional view of a further embodiment of an electrochemical sensor of the present invention formed using a recess of a base material and a sorbent material.

#### **10 Detailed Description of the Preferred Embodiment**

[0007] When used herein, the following definitions define the stated term:

[0008] An "air-oxidizable mediator" is a redox mediator that is oxidized by air, preferably so that at least 90% of the mediator is in an oxidized state upon storage in air within a useful period of time, e.g., one month or less, and, preferably, one week or less, and, more preferably, one day or less.

[0009] A "biological fluid" is any body fluid in which the analyte can be measured, for example, blood, interstitial fluid, dermal fluid, sweat, and tears.

[0010] The term "blood" in the context of the invention includes whole blood and its cell-free components, namely, plasma and serum.

[0011] "Coulometry" is the determination of charge passed or projected to pass during complete or nearly complete electrolysis of the analyte, either directly on the electrode or through one or more electron transfer agents. The charge is determined by measurement of charge passed during partial or nearly complete electrolysis of the analyte or, more often, by multiple measurements during the electrolysis of a decaying current and elapsed time. The decaying current results from the decline in the concentration of the electrolyzed species caused by the electrolysis.

[0012] A "counter electrode" refers to an electrode paired with the working electrode, through which passes an electrochemical current equal in magnitude and opposite in sign to the current passed through the working electrode. In the context of the invention, the term "counter electrode" is meant to include counter electrodes which also function as reference electrodes (i.e. a counter/reference electrode).

[0013] An "electrochemical sensor" is a device configured to detect the presence and/or measure the concentration of an analyte via electrochemical oxidation and reduction reactions on the sensor. These reactions are transduced to an electrical signal that can be correlated to an amount or concentration of analyte.

[0014] "Electrolysis" is the electrooxidation or electroreduction of a compound either directly at an electrode or via one or more electron transfer agents.

[0015] The term "facing electrodes" refers to a configuration of the working and counter electrodes in which the working surface of the working electrode is disposed in approximate opposition to a surface of the counter electrode and where the distance between the working and counter electrodes is less than the width of the working surface of the working electrode.

[0016] A compound is "immobilized" on a surface when it is entrapped on or chemically bound to the surface.

[0017] The "measurement zone" is defined herein as a region of the sample chamber sized to contain only that portion of the sample that is to be interrogated during the analyte assay.

[0018] A "non-leachable" or "non-releasable" compound is a compound which does not substantially diffuse away from the working surface of the working electrode for the duration of the analyte assay.

[0019] A "redox mediator" is an electron transfer agent for carrying electrons between the analyte and the working electrode, either directly, or via a second electron transfer agent.

[0020] A "second electron transfer agent" is a molecule which carries electrons between the redox mediator and the analyte.

[0021] "Sorbent material" is material which wicks, retains, or is wetted by a fluid sample in its void volume and which does not substantially prevent diffusion of the analyte to the electrode.

[0022] A "working electrode" is an electrode at which analyte is electrooxidized or electroreduced with or without the agency of a redox mediator.

[0023] A "working surface" is that portion of the working electrode which is coated with redox mediator and configured for exposure to sample.

[0024] The small volume, *in vitro* analyte sensors of the present invention are designed to measure the concentration of an analyte in a portion of a sample having a volume less than about 1  $\mu$ L, preferably less than about 0.5  $\mu$ L, more preferably less than about 0.2  $\mu$ L, and most preferably less than about 0.1  $\mu$ L. The analyte of interest is typically provided in a solution or biological fluid, such as blood or serum. Referring to the Drawings in general and Figures 1-4 in particular, a small volume, *in vitro* electrochemical sensor 20 of the invention generally includes a working electrode 22, a counter (or counter/reference) electrode 24, and a sample chamber 26 (see Figure 4). The sample chamber 26

is configured so that when a sample is provided in the chamber the sample is in electrolytic contact with both the working electrode 22 and the counter electrode 24. This allows electrical current to flow between the electrodes to effect the electrolysis (electrooxidation or electroreduction) of the analyte.

5      **Working Electrode**

[0025] The working electrode 22 may be formed from a molded carbon fiber composite or it may consist of an inert non-conducting base material, such as polyester, upon which a suitable conducting layer is deposited. The conducting layer should have relatively low electrical resistance and should be electrochemically inert over the potential range of 10 the sensor during operation. Suitable conductors include gold, carbon, platinum, ruthenium dioxide and palladium, as well as other non-corroding materials known to those skilled in the art. The electrode and/or conducting layers are deposited on the surface of the inert material by methods such as vapor deposition or printing.

[0026] A tab 23 may be provided on the end of the working electrode 22 for easy connection of the electrode to external electronics (not shown) such as a voltage source or current measuring equipment. Other known methods or 15 structures may be used to connect the working electrode 22 to the external electronics.

**Sensing Layer and Redox Mediator**

[0027] A sensing layer 32 containing a non-leachable (i.e., non-releasable) redox mediator is disposed on a portion 20 of the working electrode 22. Preferably, there is little or no leaching of the redox mediator away from the working electrode 22 into the sample during the measurement period, which is typically less than about 5 minutes. More preferably, the redox mediators of the present invention are bound or otherwise immobilized on the working electrode 22 to prevent undesirable leaching of the mediator into the sample. A diffusing or leachable (i.e., releasable) redox mediator is not desirable when the working and counter electrodes are close together (i.e., when the electrodes are separated 25 by less than about 1 mm), because a large background signal is typically produced as the unbound mediator shuttles electrons between the working and counter electrodes, rather than between the analyte and the working electrode. This and other problems have hindered the development of low resistance cells and increased the minimum sample size required for determination of analyte concentration.

[0028] Application of sensing layer 32 on working electrode 22 creates a working surface on that electrode. In general, 30 the working surface is that portion of the working electrode 22 coated with mediator and able to contact a fluid sample. If a portion of the sensing layer 32 is covered by a dielectric or other material, then the working surface will only be that portion of the electrode covered by redox mediator and exposed for contact with the sample.

[0029] The redox mediator mediates a current between the working electrode 22 and the analyte and enables the 35 electrochemical analysis of molecules which are not suited for direct electrochemical reaction on an electrode. The mediator functions as an electron transfer agent between the electrode and the analyte.

[0030] Almost any organic or organometallic redox species can be used as a redox mediator. In general, the preferred 40 redox mediators are rapidly reducible and oxidizable molecules having redox potentials a few hundred millivolts above or below that of the standard calomel electrode (SCE), and typically not more reducing than about -100 mV and not more oxidizing than about +400mV versus SCE. Examples of organic redox species are quinones and quinhydrone 45 and species that in their oxidized state have quinoid structures, such as Nile blue and indophenol. Unfortunately, some quinones and partially oxidized quinhydrone react with functional groups of proteins such as the thiol groups of cysteine, the amine groups of lysine and arginine, and the phenolic groups of tyrosine which may render those redox species unsuitable for some of the sensors of the present invention, e.g., sensors that will be used to measure analyte in biological fluids such as blood.

[0031] In general, mediators suitable for use in the invention have structures which prevent or substantially reduce 50 the diffusional loss of redox species during the period of time that the sample is being analyzed. The preferred redox mediators include a redox species bound to a polymer which can in turn be immobilized on the working electrode. Useful redox mediators and methods for producing them are described in U.S. Patent Nos. 5,264,104; 5,356,786; 5,262,035; and 5,320,725, herein incorporated by reference. Although, any organic or organometallic redox species can be bound to a polymer and used as a redox mediator, the preferred redox species is a transition metal compound 55 or complex. The preferred transition metal compounds or complexes include osmium, ruthenium, iron, and cobalt compounds or complexes. The most preferred are osmium compounds and complexes.

[0032] One type of non-releasable polymeric redox mediator contains a redox species covalently bound in a polymeric composition. An example of this type of mediator is poly(vinylferrocene).

[0033] Alternatively, a suitable non-releasable redox mediator contains an ionically-bound redox species. Typically, 55 these mediators include a charged polymer coupled to an oppositely charged redox species. Examples of this type of mediator include a negatively charged polymer such as Nafion® (DuPont) coupled to a positively charged redox species such as an osmium or ruthenium polypyridyl cation. Another example of an ionically-bound mediator is a positively

charged polymer such as quaternized poly(4-vinyl pyridine) or poly(1-vinyl imidazole) coupled to a negatively charged redox species such as ferricyanide or ferrocyanide.

[0034] In another embodiment of the invention, the suitable non-releasable redox mediators include a redox species coordinatively bound to the polymer. For example, the mediator may be formed by coordination of an osmium or cobalt 5 2, 2'-bipyridyl complex to poly(1-vinyl imidazole) or poly(4-vinyl pyridine).

[0035] The preferred redox mediators are osmium transition metal complexes with one or more ligands having a nitrogen-containing heterocycle such as 2,2'-bipyridine, 1,10-phenanthroline or derivatives thereof. Furthermore, the preferred redox mediators also have one or more polymeric ligands having at least one nitrogen-containing heterocycle, such as pyridine, imidazole, or derivatives thereof. These preferred mediators exchange electrons rapidly between 10 each other and the electrodes so that the complex can be rapidly oxidized and reduced.

[0036] In particular, it has been determined that osmium cations complexed with two ligands containing 2,2'-bipyridine, 1,10-phenanthroline, or derivatives thereof, the two ligands not necessarily being the same, and further complexed with a polymer having pyridine or imidazole functional groups form particularly useful redox mediators in the small 15 volume sensors of the present invention. Preferred derivatives of 2,2'-bipyridine for complexation with the osmium cation are 4,4'-dimethyl-2,2'-bipyridine and mono-, di-, and polyalkoxy-2,2'-bipyridines, such as 4,4'-dimethoxy-2,2'-bipyridine, where the carbon to oxygen ratio of the alkoxy groups is sufficient to retain solubility of the transition metal complex in water. Preferred derivatives of 1,10-phenanthroline for complexation with the osmium cation are 4,7-dimethyl-1,10-phenanthroline and mono-, di-, and polyalkoxy-1,10-phenanthrolines, such as 4,7-dimethoxy-1,10-phenanthroline, where the carbon to oxygen ratio of the alkoxy groups is sufficient to retain solubility of the transition metal 20 complex in water. Preferred polymers for complexation with the osmium cation include poly(1-vinyl imidazole), e.g., PVI, and poly(4-vinyl pyridine), e.g., PVP, either alone or with a copolymer. Most preferred are redox mediators with osmium complexed with poly(1-vinyl imidazole) alone or with a copolymer.

[0037] The preferred redox mediators have a redox potential between about -150 mV to about +400 mV versus the standard calomel electrode (SCE). Preferably, the potential of the redox mediator is between about -100 mV and +100 mV and more preferably, the potential is between about -50 mV and +50 mV. The most preferred redox mediators have 25 osmium redox centers and a redox potential more negative than +100 mV versus SCE, more preferably the redox potential is more negative than +50 mV versus SCE, and most preferably is near -50 mV versus SCE.

[0038] It is also preferred that the redox mediators of the inventive sensors be air-oxidizable. This means that the redox mediator is oxidized by air, preferably so that at least 90% of the mediator is in an oxidized state prior to introduction of sample into the sensor. Air-oxidizable redox mediators include osmium cations complexed with two mono-, di-, or polyalkoxy-2,2'-bipyridine or mono-, di-, or polyalkoxy-1,10-phenanthroline ligands, the two ligands not necessarily being the same, and further complexed with polymers having pyridine and imidazole functional groups. In particular,  $\text{Os}[4,4'\text{-dimethoxy-2,2'-bipyridine}]_2\text{Cl}^{+/-2}$  complexed with poly(4-vinyl pyridine) or poly(1-vinyl imidazole) attains approximately 90% or more oxidation in air.

[0039] In a preferred embodiment of the invention, the sensing layer 32 includes a second electron transfer agent which is capable of transferring electrons to or from the redox mediator and the analyte. One example of a suitable second electron transfer agent is an enzyme which catalyzes a reaction of the analyte. For example, a glucose oxidase or glucose dehydrogenase, such as pyrroloquinoline quinone glucose dehydrogenase (PQQ), is used when the analyte is glucose. A lactate oxidase fills this role when the analyte is lactate. These enzymes catalyze the electrolysis of an 30 analyte by transferring electrons between the analyte and the electrode via the redox mediator. Preferably, the second electron transfer agent is non-leachable, and more preferably immobilized on the electrode, to prevent unwanted leaching of the agent into the sample. This is accomplished, for example, by cross linking the second electron transfer agent with the redox mediator, thereby providing a sensing layer with non-leachable components.

[0040] To prevent electrochemical reactions from occurring on portions of the working electrode not coated by the 45 mediator, a dielectric 40 may be deposited on the electrode over, under, or surrounding the region with the bound redox mediator, as shown in Figure 4. Suitable dielectric materials include waxes and non-conducting organic polymers such as polyethylene. Dielectric 40 may also cover a portion of the redox mediator on the electrode. The covered portion of the mediator will not contact the sample, and, therefore, will not be a part of the electrode's working surface.

## 50 Counter Electrode

[0041] Counter electrode 24 may be constructed in a manner similar to working electrode 22. Counter electrode 24 55 may also be a counter/reference electrode. Alternatively, a separate reference electrode may be provided in contact with the sample chamber. Suitable materials for the counter/reference or reference electrode include Ag/AgCl printed on a non-conducting base material or silver chloride on a silver metal base. If the counter electrode is not a reference electrode, the same materials and methods may be used to make the counter electrode as are available for constructing the working electrode 22, however, no redox mediator is immobilized on the counter or counter/reference electrode 24. A tab 25 may be provided on the electrode for convenient connection to the external electronics (not shown), such

as a coulometer or other measuring device.

[0042] In one embodiment of the invention, working electrode 22 and counter electrode 24 are disposed opposite to and facing each other to form a facing electrode pair as depicted in Figures 1 and 3. In this preferred configuration, the sample chamber 26 is typically disposed between the two electrodes. For this facing electrode configuration, it is preferred that the electrodes are separated by a distance of less than about 0.2mm, preferably less than 0.1 mm, and most preferably less than 0.05 mm.

[0043] The electrodes need not be directly opposing each other, they may be slightly offset. Furthermore, the two electrodes need not be the same size. Preferably, the counter electrode 24 is at least as large as the working surface of the working electrode 22. The counter electrode 22 can also be formed with tines in a comb shape. Other configuration of both the counter electrode and working electrode are within the scope of the invention. However, the separation distance between any portion of the working electrode and some portion of the counter electrode preferably does not exceed the limits specified hereinabove.

[0044] Figures 11A, 11B, and 11C illustrate different embodiments of pairs of facing electrodes 22, 24, as described above. A region 21 of overlap between the two electrodes 22, 24 typically corresponds to the measurement zone in which the sample will be interrogated. Each of the electrodes 22, 24 is a conducting surface and acts as a plate of a capacitor. The measurement zone between the electrodes 22, 24 acts as a dielectric layer between the plates. Thus, there is a capacitance between the two electrodes 22, 24. This capacitance is a function of the size of the overlapping electrodes 22, 24, the separation between the electrodes 22, 24, and the dielectric constant of the material between the electrodes 22, 24. Thus, if the size of the region 21 of the overlapping electrodes 22, 24 and the dielectric constant of the material between the electrodes (e.g., air or a sorbent material) are known, then the separation between the electrodes can be calculated to determine the volume of the measurement zone.

[0045] Figure 11A illustrates one embodiment of the invention in which the electrodes 22, 24 are positioned in a facing arrangement. For the capacitance to be uniform among similarly constructed analyte sensors having this particular sensor configuration, the registration (i.e., the positioning of the two electrodes relative to one another) should be uniform. If the position of either of the electrodes is shifted in the x-y plane from the position shown in Figure 11A, the size of the overlap, and therefore, of the capacitance, will change. The same principle holds for the volume of the measurement zone.

[0046] Figures 11B and 11C illustrate other embodiments of the invention with electrodes 22, 24 in a facing arrangement. In these particular arrangements, the position of either of the electrodes may be shifted, by at least some minimum distance, in the x-y plane relative to the other electrode without a change in the capacitance or the volume of the measurement zone. In these electrode arrangements, each electrode 22, 24 includes an arm 122, 124, respectively, which overlaps with the corresponding arm of the other electrode. The two arms 122, 124 are not parallel to each other (such as illustrated in Figure 11A); rather, the arms 122, 124 are disposed at an angle 123, which is greater than zero, relative to each other. In addition, the two arms 122, 124 extend beyond the region 21 of overlap (i.e., each arm has extra length corresponding to the difference between the length of the arm 222, 224, respectively, and the width 121 of the overlap 21). With these electrode arrangements, there can be a certain amount of allowed imprecision in the registration of the electrodes 22, 24 which does not change the capacitance of the electrode arrangement. A desired amount of allowed imprecision in the registration can be designed into the electrode arrangement by varying the angle 123 at which the arms 122, 124 overlap and the size of the extra length of each arm 122, 124 relative to the width 121 of the region 21 of overlap. Typically, the closer that the arms 122, 124 are to being perpendicular (i.e., angle 123 is 90°), the greater the allowed imprecision. Also, the greater the extra length of each arm 122, 124 (which may both be the same length or different lengths) relative to the width 121 of the region 21 of overlap, the greater the allowed imprecision. Conversely, the greater the amount of allowed imprecision, the larger the size of the electrodes (for a given electrode width, thickness, and angle 123 of intersection with the other electrode). Thus, the minimum distance that one electrode can be shifted relative to the other is balanced against the amount of material needed for the electrodes. Typically, the angle 123 of intersection ranges from 5 to 90 degrees, preferably, 30 to 90 degrees, and more preferably 60 to 90 degrees. Typically, the ratio of the extra length of an arm 122, 124 (corresponding to the difference between the arm length 222, 224 and the width 121 of the region 21 of overlap) versus the width 121 of the region 21 of overlap ranges from 0.1:1 to 50:1, preferably 1:1 to 15:1, and more preferably 4:1 to 10:1.

[0047] In another embodiment of the invention, the two electrodes 22, 24 are coplanar as shown in Figure 2. In this case, the sample chamber 26 is in contact with both electrodes and is bounded on the side opposite the electrodes by a non-conducting inert base 30. Suitable materials for the inert base include non-conducting materials such as polyester.

[0048] Other configurations of the inventive sensors are also possible. For example, the two electrodes may be formed on surfaces that make an angle to each other. One such configuration would have the electrodes on surfaces that form a right angle. Another possible configuration has the electrodes on a curved surface such as the interior of a tube. The working and counter electrodes may be arranged so that they face each other from opposite sides of the tube. This is another example of a facing electrode pair. Alternatively, the electrodes may be placed near each other

on the tube wall (e.g., one on top of the other or side-by-side).

[0049] In any configuration, the two electrodes must be configured so that they do not make direct electrical contact with each other, to prevent shorting of the electrochemical sensor. This may be difficult to avoid when the facing electrodes having a short (less than about 100 $\mu\text{m}$ ) distance between them.

5 [0050] A spacer 28 can be used to keep the electrodes apart when the electrodes face each other as depicted in Figures 1 and 3. The spacer is typically constructed from an inert non-conducting material such as polyester, Mylar™, Kevlar™ or any other strong, thin polymer film, or, alternatively, a thin polymer film such as a Teflon™ film, chosen for its chemical inertness. In addition to preventing contact between the electrodes, the spacer 28 often functions as a portion of the boundary for the sample chamber 26 as shown in Figures 1-4.

10

### Sample Chamber

15 [0051] The sample chamber 26 is typically defined by a combination of the electrodes 22, 24, an inert base 30, and a spacer 28 as shown in Figures 1-4. A measurement zone is contained within this sample chamber and is the region of the sample chamber that contains only that portion of the sample that is interrogated during the analyte assay. In the embodiment of the invention illustrated in Figures 1 and 2, sample chamber 26 is the space between the two electrodes 22, 24 and/or the inert base 30. In this embodiment, the sample chamber has a volume that is preferably less than about 1  $\mu\text{L}$ , more preferably less than about 0.5  $\mu\text{L}$ , and most preferably less than about 0.2  $\mu\text{L}$ . In the embodiment of the invention depicted in Figures 1 and 2, the measurement zone has a volume that is approximately equal to the volume of the sample chamber.

20 [0052] In another embodiment of the invention, shown in Figure 3, sample chamber 26 includes much more space than the region proximate electrodes 22, 24. This configuration makes it possible to provide multiple electrodes in contact with one or more sample chambers, as shown in Figure 5. In this embodiment, sample chamber 26 is preferably sized to contain a volume of less than about 1  $\mu\text{L}$ , more preferably less than about 0.5  $\mu\text{L}$ , and most preferably less than about 0.2  $\mu\text{L}$ . The measurement zone (i.e., the region containing the volume of sample to be interrogated) is generally sized to contain a volume of sample of less than about 1  $\mu\text{L}$ , preferably less than about 0.5  $\mu\text{L}$ , more preferably less than about 0.2  $\mu\text{L}$ , and most preferably less than about 0.1  $\mu\text{L}$ . One particularly useful configuration of this embodiment positions working electrode 22 and counter electrode 24 facing each other, as shown in Figure 3. In this embodiment, the measurement zone, corresponding to the region containing the portion of the sample which will be interrogated, is the portion of sample chamber 26 bounded by the working surface of the working electrode and disposed between the two facing electrodes. When the surface of the working electrode is not entirely covered by redox mediator, the measurement zone is the space between the two facing electrodes that has a surface area corresponding to the working surface (i.e., redox mediator-covered surface) of working electrode 22 and a thickness corresponding to the separation distance between working electrode 22 and counter electrode 24.

25 [0053] In both of the embodiments discussed above, the thickness of the sample chamber and of the measurement zone correspond typically to the thickness of spacer 28 (e.g., the distance between the electrodes in Figures 1 and 3, or the distance between the electrodes and the inert base in Figure 2). Preferably, this thickness is small to promote rapid electrolysis of the analyte, as more of the sample will be in contact with the electrode surface for a given sample volume. In addition, a thin sample chamber helps to reduce errors from diffusion of analyte into the measurement zone from other portions of the sample chamber during the analyte assay, because diffusion time is long relative to the measurement time. Typically, the thickness of the sample chamber is less than about 0.2 mm. Preferably, the thickness of the sample chamber is less than about 0.1 mm and, more preferably, the thickness of the sample chamber is about 0.05 mm or less.

30 [0054] The sample chamber may be formed by other methods. Exemplary methods include embossing, indenting, or otherwise forming a recess in a substrate within which either the working electrode 22 or counter electrode 24 is formed. Figures 12A and 12B illustrate one embodiment of this structure. First, a conducting layer 100 is formed on an inert non-conducting base material 102. As described above, the conducting layer 100 can include gold, carbon, platinum, ruthenium dioxide, palladium, or other non-corroding materials. The inert non-conducting base material 102 can be made using a polyester, other polymers, or other non-conducting, deformable materials. A recess 104 is then formed in a region of the non-conducting base material 102 so that at least a portion of the conducting layer 100 is included in the recess 104. The recess 104 may be formed using a variety of techniques including indenting, deforming, or otherwise pushing in the base material 102. One additional exemplary method for forming the recess includes embossing the base material 102. For example, the base material 102 may be brought into contact with an embossing roll or stamp having raised portions, such as punch members or channels, to form the recess 104. In some embodiments, the base material 102 may be heated to soften the material.

35 [0055] The recess 104 may be circular, oval, rectangular, or any other regular or irregular shape. Alternatively, the recess 104 may be formed as a channel which extends along a portion of the base material 102. The conducting layer 100 may extend along the entire channel or only a portion of the channel. The measurement zone may be restricted

to a particular region within the channel by, for example, depositing the sensing layer 32 on only that portion of the conducting layer 100 within the particular region of the channel. Alternatively, the measurement zone may be defined by placing a second electrode 107 over only the desired region of the first electrode 105.

[0056] At least a portion, and in some cases, all, of the conducting layer 100 is situated in the recess 104. This portion of the conducting layer 100 may act as a first electrode 105 (a counter electrode or, preferably, a working electrode). If the conducting layer 100 forms the working electrode, then a sensing layer 32 may be formed over a portion of the conducting layer 100 by depositing the non-leachable mediator and optional second electron transfer agent in the recess 104, as shown in Figure 12B. A second electrode 107 is then formed by depositing a second conducting layer on a second base material 106. This second electrode 107 is then positioned over the first electrode 105 in a facing arrangement. Although not illustrated, it will be understood that if the first electrode 105 were to function as a counter electrode, then the sensing layer 32 would be deposited on the second electrode 107 which would then function as the working electrode.

[0057] In one embodiment, the second base material 108 rests on a portion of the first base material 102 and/or the conducting layer 100 which is not depressed, so that the second electrode 107 extends into the recess. In another embodiment, there is a spacer (not shown) between the first and second base materials 102, 108. In this embodiment, the second electrode 107 may or may not extend into the recess. In any case, the first and second electrodes 105, 107 do not make contact, otherwise the two electrodes would be shorted.

[0058] The depth of the recess 104 and the volume of the conductive layer 100, sensing layer 32, and the portion, if any, of the second electrode 107 in the recess 104 determines the volume of the measurement zone. Thus, the predictability of the volume of the measurement zone relies on the extent to which the formation of the recess 104 is uniform.

[0059] In addition to the conducting layer 100, a sorbent layer 103, described in detail below, may be deposited on the base material 102 prior to forming the recess 104, as shown in Figure 14A. The sorbent material 103 may be indented, embossed, or otherwise deformed with the conducting layer 100 and base material 102, as shown in Figure 14B. Alternatively, the sorbent material 103 may be deposited after the conducting layer 100 and base material 102 are indented, embossed, or otherwise deformed to make the recess 104.

[0060] In another exemplary method for forming the analyte sensor. A recess 114 is formed in a first base material 112, as shown in Figures 13A and 13B. The recess may be formed by indenting, embossing, etching (e.g., using photolithographic methods or laser removal of a portion of the base material), or otherwise deforming or removing a portion of the base material 112. Then a first conducting layer 110 is formed in the recess 114. Any of the conductive materials discussed above may be used. A preferred material is a conductive ink, such as a conductive carbon ink available, for example, from Ercon, Inc. (Wareham, MA). The conductive ink typically contains metal or carbon dissolved or dispersed in a solvent or dispersant. When the solvent or dispersant is removed, the metal or carbon forms a conductive layer 110 that can then be used as a first electrode 115. A second electrode 117 can be formed on a second base material 116 and positioned over the recess 114, as described above. In some embodiments, a sensing layer 32 is formed on the first electrode 115 to form a working electrode, as shown in Figure 13B. In other embodiments, the sensing layer 32 may be formed on the second electrode 117 to form a working electrode. Furthermore, a sorbent material (not shown) may be formed within the recess, for example, on the first electrode 115.

[0061] A binder, such as a polyurethane resin, cellulose derivative, elastomer (e.g., silicones, polymeric dienes, or acrylonitrile-butadiene-styrene (ABS) resins), highly fluorinated polymers, or the like, may also be included in the conductive ink. Curing the binder may increase the conductivity of the conductive layer 110, however, curing is not necessary. The method of curing the binder may depend on the nature of the particular binder that is used. Some binders are cured by heat and/or ultraviolet light.

[0062] These structures allow for the formation of electrochemical sensors in which the volume of the measurement zone depends, at least in part, on the accuracy and reproducibility of the recess 104. Embossing, laser etching, photolithographic etching and other methods can be used to make reproducible recesses 104, even on the scale of 200  $\mu\text{m}$  or less.

#### Sorbent Material

[0063] The sample chamber may be empty before the sample is placed in the chamber. Alternatively, the sample chamber may include a sorbent material 34 to sorb and hold a fluid sample during the measurement process. Suitable sorbent materials include polyester, nylon, cellulose, and cellulose derivatives such as nitrocellulose. The sorbent material facilitates the uptake of small volume samples by a wicking action which may complement or, preferably, replace any capillary action of the sample chamber.

[0064] In some embodiments, the sorbent material is deposited using a liquid or slurry in which the sorbent material is dissolved or dispersed. The solvent or dispersant in the liquid or slurry may then be driven off by heating or evaporation processes. Suitable sorbent materials include, for example, cellulose or nylon powders dissolved or dispersed in a

suitable solvent or dispersant, such as water. The particular solvent or dispersant should also be compatible with the material of the working electrode 22 (e.g., the solvent or dispersant should not dissolve the electrode.)

**[0065]** One of the most important functions of the sorbent material is to reduce the volume of fluid needed to fill the sample chamber and corresponding measurement zone of the sensor. The actual volume of sample within the measurement zone is partially determined by the amount of void space within the sorbent material. Typically, suitable sorbents consist of about 5% to about 50% void space. Preferably, the sorbent material consists of about 10% to about 25% void space.

**[0066]** The displacement of fluid by the sorbent material is advantageous. By addition of a sorbent, less sample is needed to fill sample chamber 26. This reduces the volume of sample that is required to obtain a measurement and also reduces the time required to electrolyze the sample.

**[0067]** The sorbent material 34 may include a tab 33 which is made of the same material as the sorbent and which extends from the sensor, or from an opening in the sensor, so that a sample may be brought into contact with tab 33, sorbed by the tab, and conveyed into the sample chamber 26 by the wicking action of the sorbent material 34. This provides a preferred method for directing the sample into the sample chamber 26. For example, the sensor may be brought into contact with a region of an animal (including human) that has been pierced with a lancet to draw blood. The blood is brought in contact with tab 33 and drawn into sample chamber 26 by the wicking action of the sorbent 34. The direct transfer of the sample to the sensor is especially important when the sample is very small, such as when the lancet is used to pierce a portion of the animal that is not heavily supplied with near-surface capillary vessels and furnishes a blood sample volume of less than 1  $\mu\text{L}$ .

**[0068]** Methods other than the wicking action of a sorbent may be used to transport the sample into the sample chamber or measurement zone. Examples of such means for transport include the application of pressure on a sample to push it into the sample chamber, the creation of a vacuum by a pump or other vacuum-producing means in the sample chamber to pull the sample into the chamber, capillary action due to interfacial tension of the sample with the walls of a thin sample chamber, as well as the wicking action of a sorbent material.

**[0069]** The sensor can also be used in conjunction with a flowing sample stream. In this configuration, the sample stream is made to flow through a sample chamber. The flow is stopped periodically and the concentration of the analyte is determined by electrochemical method, such as coulometry. After the measurement, the flow is resumed, thereby removing the sample from the sensor. Alternatively, sample may flow through the chamber at a very slow rate, such that all of the analyte is electrolyzed in transit, yielding a current dependent only upon analyte concentration and flow rate.

**[0070]** Other filler materials may be used to fill the measurement zone and reduce the sample volume. For example, glass beads can be deposited in the measurement zone to occupy space. Preferably, these filler materials are hydrophilic so that the body fluid can easily flow into the measurement zone. In some cases, such as glass beads with a high surface area, these filler materials may also wick the body fluid into the measurement zone due to their high surface area and hydrophilicity.

**[0071]** The entire sensor assembly is held firmly together to ensure that the sample remains in contact with the electrodes and that the sample chamber and measurement zone maintain the same volume. This is an important consideration in the coulometric analysis of a sample, where measurement of a defined sample volume is needed. One method of holding the sensor together is depicted in Figures 1 and 2. Two plates 38 are provided at opposite ends of the sensor. These plates are typically constructed of non-conducting materials such as plastics. The plates are designed so that they can be held together with the sensor between the two plates. Suitable holding devices include adhesives, clamps, nuts and bolts, screws, and the like.

#### Integrated Sample Acquisition and Analyte Measurement Device



**[0072]** In a preferred embodiment of the invention, an analyte measurement device 52 constructed according to the principles of the present invention includes a sensor 20, as described hereinabove, combined with a sample acquisition means 50 to provide an integrated sampling and measurement device. The sample acquisition means 50 illustrated in Figure 6, includes, for example, a skin piercing member 54, such as a lancet, attached to a resilient deflectable strip 56 (or other similar device, such as a spring) which may be pushed to inject the lancet into a patient's skin to cause blood flow.

**[0073]** The resilient strip 56 is then released and the skin piercing member 54 retracts. Blood flowing from the area of skin pierced by member 54 can then be transported, for example, by the wicking action of sorbent material 34, into sensor 20 for analysis of the analyte. The analyte measurement device 52 may then be placed in a reader, not shown, which connects a coulometer or other electrochemical analysis equipment to the electrode tabs 23, 25 to determine the concentration of the analyte by electroanalytical means.

**Operation of the Sensor**

[0074] An electrochemical sensor of the invention is operated in the following manner. A potential is applied across the working and counter electrodes. The magnitude of the required potential is dependent on the redox mediator. The potential at an electrode where the analyte is electrolyzed is typically large enough to drive the electrochemical reaction to or near completion, but the magnitude of the potential is, preferably, not large enough to induce significant electrochemical reaction of interferents, such as urate, ascorbate, and acetaminophen, that may affect the current measurements. Typically the potential is between about -150 mV and about +400 mV versus the standard calomel electrode (SCE). Preferably, the potential of the redox mediator is between about -100 mV and +100 mV and, more preferably, the potential is between about -50 mV and +50 mV.

[0075] The potential may be applied either before or after the sample has been placed in the sample chamber. The potential is preferably applied after the sample has come to rest in the sample chamber to prevent electrolysis of sample passing through the measurement zone as the sample chamber is filling. When the potential is applied and the sample is in the measurement zone, an electrical current will flow between the working electrode and the counter electrode. The current is a result of the electrolysis of the analyte in the sample. This electrochemical reaction occurs via the redox mediator and the optional second electron transfer agent. For many biomolecules, B, the process is described by the following reaction equations:



Biochemical B is oxidized to C by redox mediator species A in the presence of an appropriate enzyme. Then the redox mediator A is oxidized at the electrode. Electrons are collected by the electrode and the resulting current is measured.

[0076] As an example, one sensor of the present invention is based on the reaction of a glucose molecule with two non-leachable ferricyanide anions in the presence of glucose oxidase to produce two non-leachable ferrocyanide anions, two protons and gluconolactone. The amount of glucose present is assayed by electrooxidizing the non-leachable ferrocyanide anions to non-leachable ferricyanide anions and measuring the total charge passed.

[0077] Those skilled in the art will recognize that there are many different reaction mechanisms that will achieve the same result; namely the electrolysis of an analyte through a reaction pathway incorporating a redox mediator. Equations (1) and (2) are a non-limiting example of such a reaction.

[0078] In a preferred embodiment of the invention, coulometry is used to determine the concentration of the analyte. This measurement technique utilizes current measurements obtained at intervals over the course of the assay, to determine analyte concentration. These current measurements are integrated over time to obtain the amount of charge, Q, passed to or from the electrode. Q is then used to calculate the concentration of the analyte by the following equation:

$$[\text{analyte}] = Q/nFV \quad (3)$$

where n is the number of electron equivalents required to electrolyze the analyte, F is Faraday's constant (approximately 96,500 coulombs per equivalent), and V is the volume of sample in the measurement zone.

[0079] In one embodiment of the invention, the analyte is completely or nearly completely electrolyzed. The charge is then calculated from current measurements made during the electrochemical reaction and the concentration of the analyte is determined using equation (3). The completion of the electrochemical reaction is typically signaled when the current reaches a steady-state value. This indicates that all or nearly all of the analyte has been electrolyzed. For this type of measurement, at least 90% of the analyte is typically electrolyzed, preferably, at least 95% of the analyte is electrolyzed and, more preferably, at least 99% of the analyte is electrolyzed.

[0080] For this method it is desirable that the analyte be electrolyzed quickly. The speed of the electrochemical reaction depends on several factors, including the potential that is applied between the electrodes and the kinetics of reactions (1) and (2). (Other significant factors include the size of the measurement zone and the presence of sorbent in the measurement zone.) In general, the larger the potential, the larger the current through the cell (up to a transport limited maximum) and therefore, the faster the reaction will typically occur. However, if the potential is too large, other electrochemical reactions may introduce significant error in the measurement. Typically, the potential between the

electrodes as well as the specific redox mediator and optional second electron transfer agent are chosen so that the analyte will be almost completely electrolyzed in less than 5 minutes, based on the expected concentration of the analyte in the sample. Preferably, the analyte will be almost completely electrolyzed within about 2 minutes and, more preferably, within about 1 minute.

5 [0081] In another embodiment of the invention, the analyte is only partially electrolyzed. The current is measured during the partial reaction and then extrapolated using mathematical techniques known to those skilled in the art to determine the current curve for the complete or nearly complete electrolysis of the analyte. Integration of this curve yields the amount of charge that would be passed if the analyte were completely or nearly completely electrolyzed and, using equation (3), the concentration of the analyte is calculated.

10 [0082] The above described methods are based on coulometric analyses, due to the advantages of coulometric measurements, as described hereinbelow. However, those skilled in the art will recognize that a sensor of the invention may also utilize potentiometric, amperometric, voltammetric, and other electrochemical techniques to determine the concentration of an analyte in a sample. There are, however, disadvantages to using some of these techniques. The measurements obtained by these non-coulometric methods are not temperature independent as the current and potential obtained by the electrolysis of an analyte on an electrode is very sensitive to sample temperature. This presents a problem for the calibration of a sensor which will be used to measure bioanalytes and other samples at unknown or variable temperatures.

15 [0083] In addition, the measurements obtained by these non-coulometric electrochemical techniques are sensitive to the amount of enzyme provided in the sensor. If the enzyme deactivates or decays over time, the resulting measurements will be affected. This will limit the shelf life of such sensors unless the enzyme is very stable.

20 [0084] Finally, the measurements obtained by non-coulometric electrochemical techniques such as amperometry will be negatively affected if a substantial portion of the analyte is electrolyzed during the measurement period. An accurate steady-state measurement can not be obtained unless there is sufficient analyte so that only a relatively small portion of the analyte is electrolyzed during the measurement process.

25 [0085] The electrochemical technique of coulometry overcomes these problems. Coulometry is a method for determining the amount of charge passed or projected to pass during complete or nearly complete electrolysis of the analyte. One coulometric technique involves electrolyzing the analyte on a working electrode and measuring the resulting current between the working electrode and a counter electrode at two or more times during the electrolysis. The electrolysis is complete when the current reaches a steady state. The charge used to electrolyze the sample is then calculated by integrating the measured currents over time. Because the charge is directly related to the amount of analyte in the sample there is no temperature dependence of the measurement. In addition, the activity of the redox mediator does not affect the value of the measurement, but only the time required to obtain the measurement (i.e., less active redox mediator requires a longer time to achieve complete electrolysis of the sample) so that decay of the mediator over time will not render the analyte concentration determination inaccurate. And finally, the depletion of the analyte in the sample by electrolysis is not a source of error, but rather the objective of the technique. (However, the analyte need not be completely electrolyzed if the electrolysis curve is extrapolated from the partial electrolysis curve based on well-known electrochemical principles.)

30 [0086] For coulometry to be an effective measurement technique for determining the concentration of an analyte in a sample, it is necessary to accurately determine the volume of the measured sample. Unfortunately, the volume of the sample in the measurement zone of a small volume sensor (i.e., less than one microliter) may be difficult to accurately determine because the manufacturing tolerances of one or more dimensions of the measurement zone may have significant variances.

#### Air-oxidizable Redox Mediators

35 [0087] Another source of error in a coulometric sensor is the presence of electrochemical reactions other than those associated with the analyte. In a sensor having a redox mediator, a potential source of measurement error is the presence of redox mediator in an unknown mixed oxidation state (i.e., mediator not reproducibly in a known oxidation state). Redox mediator will then be electrolyzed at the electrode, not in response to the presence of an analyte, but simply due to its initial oxidation state. Referring to equations (1) and (2), current not attributable to the oxidation of biochemical B will flow due to oxidation of a portion of a redox mediator, A, that is in its reduced form prior to the addition of the sample. Thus, it is important to know the oxidation state of the analyte prior to introduction of the sample into the sensor. Furthermore, it is desirable that all or nearly all of the redox mediator be in a single oxidation state prior to the introduction of the sample into the sensor.

40 [0088] Each redox mediator has a reduced form or state and an oxidized form or state. In one aspect of the invention, it is preferred that the amount of redox mediator in the reduced form prior to the introduction of sample be significantly smaller than the expected amount of analyte in a sample in order to avoid a significant background contribution to the measured current. In this embodiment of the invention, the molar amount of redox mediator in the reduced form prior

to the introduction of the analyte is preferably less than, on a stoichiometric basis, about 10%, and more preferably less than about 5%, and most preferably less than 1%, of the molar amount of analyte for expected analyte concentrations. (The molar amounts of analyte and redox mediator should be compared based on the stoichiometry of the applicable redox reaction so that if two moles of redox mediator are needed to electrolyze one mole of analyte, then the molar amount of redox mediator in the reduced form prior to introduction of the analyte is preferably less than 20% and more preferably less than about 10% and most preferably less than about 2% of the molar amount of analyte for expected analyte concentrations.) Methods for controlling the amount of reduced mediator are discussed below.

[0089] In another aspect of the invention, it is preferred that the relative ratio of oxidized redox mediator to reduced redox mediator prior to introduction of the sample in the sensor be relatively constant between similarly constructed sensors. The degree of variation in this ratio between similarly constructed sensors will negatively affect the use of a calibration curve to account for the reduced mediator, as significant variations between sensors will make the calibration less reliable. For this aspect of the invention, the percentage of the redox mediator in the reduced form prior to introduction of the sample in the sensor varies by less than about 20% and preferably less than about 10% between similarly constructed sensors.

[0090] One method of controlling the amount of reduced redox mediator prior to the introduction of the sample in the sensor is to provide an oxidizer to oxidize the reduced form of the mediator. One of the most convenient oxidizers is O<sub>2</sub>. Oxygen is usually readily available to perform this oxidizing function. Oxygen can be supplied by exposing the sensor to air. In addition, most polymers and fluids absorb O<sub>2</sub> from the air unless special precautions are taken. Typically, at least 90% of an air-oxidizable (i.e., O<sub>2</sub> oxidizable) mediator is in the oxidized state upon storage or exposure to air for a useful period of time, e.g., one month or less, and preferably, one week or less, and, more preferably, one day or less.

[0091] Suitable mediators which are both air-oxidizable (i.e., O<sub>2</sub>-oxidizable) and have electron transfer capabilities have been described hereinabove. One particular family of useful mediators are osmium complexes which are coordinated or bound to ligands with one or more nitrogen-containing heterocycles. In particular, osmium complexed with mono-, di-, and polyalkoxy-2,2'-bipyridine or mono-, di-, and polyalkoxy-1,10-phenanthroline, where the alkoxy groups have a carbon to oxygen ratio sufficient to retain solubility in water, are air-oxidizable. These osmium complexes typically have two substituted bipyridine or substituted phenanthroline ligands, the two ligands not necessarily being identical. These osmium complexes are further complexed with a polymeric ligand with one or more nitrogen-containing heterocycles, such as pyridine and imidazole. Preferred polymeric ligands include poly(4-vinyl pyridine) and, more preferably, poly(1-vinyl imidazole) or copolymers thereof. Os[4,4'-dimethoxy-2,2'-bipyridine]<sub>2</sub>Cl<sup>+/+2</sup> complexed with a poly(1-vinyl imidazole) or poly(4-vinyl pyridine) has been shown to be particularly useful as the Os<sup>+2</sup> cation is oxidizable by O<sub>2</sub> to Os<sup>+3</sup>. Similar results are expected for complexes of Os[4,7-dimethoxy-1,10-phenanthroline]<sub>2</sub>Cl<sup>+/+2</sup>, and other mono-, di-, and polyalkoxy bipyridines and phenanthrolines, with the same polymers.

[0092] A complication associated with air-oxidizable mediators arises if the air oxidation of the redox mediator is so fast that a substantial portion of the analyte-reduced redox mediator is oxidized by O<sub>2</sub> during an analyte assay. This will result in an inaccurate assay as the amount of analyte will be underestimated because the mediator will be oxidized by the oxidizer rather than by electrooxidation at the electrode. Thus, it is preferred that the reaction of the redox mediator with O<sub>2</sub> proceeds more slowly than the electrooxidation of the mediator. Typically, less than 5%, and preferably less than 1%, of the reduced mediator should be oxidized by the oxidizer during an assay.

[0093] The reaction rate of the air oxidation of the mediator can be controlled through choice of an appropriate complexing polymer. For example, the oxidation reaction is much faster for Os[4,4'-dimethoxy-2,2'-bipyridine]<sub>2</sub>Cl<sup>+/+2</sup> coordinatively coupled to poly(1-vinyl imidazole) than for the same Os complex coupled to poly(4-vinyl pyridine). The choice of an appropriate polymer will depend on the expected analyte concentration and the potential applied between the electrodes, both of which determine the rate of the electrochemical reaction.

[0094] Thus, in one embodiment of the invention, the preferred redox mediator has the following characteristics: 1) the mediator does not react with any molecules in the sample or in the sensor other than the analyte (optionally, via a second electron transfer agent); 2) nearly all of the redox mediator is oxidized by an oxidizer such as O<sub>2</sub> prior to introduction of the sample in the sensor; and 3) the oxidation of the redox mediator by the oxidizer is slow compared to the electrooxidation of the mediator by the electrode.

[0095] Alternatively, if the redox mediator is to be oxidized in the presence of the analyte and electroreduced at the electrode, a reducer rather than an oxidizer would be required. The same considerations for the appropriate choice of reducer and mediator apply as described hereinabove for the oxidizer.

[0096] The use of stable air-oxidizable redox mediators in the electrochemical sensors of the invention provides an additional advantage during storage and packaging. Sensors of the invention which include air oxidizable redox mediators can be packaged in an atmosphere containing molecular oxygen and stored for long periods of time, e.g., greater than one month, while maintaining more than 80% and preferably more than 90% of the redox species in the oxidized state.

**Optical Sensors**

[0097] The air-oxidizable redox species of the present invention can be used in other types of sensors. The osmium complexes described hereinabove are suitable for use in optical sensors, due to the difference in the absorption spectra and fluorescence characteristics of the complexed Os<sup>+2</sup> and Os<sup>+3</sup> species. Absorption, transmission, reflection, or fluorescence measurements of the redox species will correlate with the amount of analyte in the sample (after reaction between an analyte and the redox species, either directly, or via a second electron transfer agent such as an enzyme). In this configuration, the molar amount of redox mediator should be greater, on a stoichiometric basis, than the molar amount of analyte reasonably expected to fill the measurement zone of the sensor.

[0098] Standard optical sensors, including light-guiding optical fiber sensors, and measurement techniques can be adapted for use with the air-oxidizable mediators. For example, the optical sensors of the invention may include a light-transmitting or light reflecting support on which the air-oxidizable redox species, and preferably an analyte-responsive enzyme, is coated to form a film. The support film forms one boundary for the measurement zone in which the sample is placed. The other boundaries of the measurement zone are determined by the configuration of the cell. Upon filling the measurement zone with an analyte-containing sample, reduction of the air-oxidizable mediator by the analyte, preferably via reaction with the analyte-responsive enzyme, causes a shift in the mediator's oxidation state that is detected by a change in the light transmission, absorption, or reflection spectra or in the fluorescence of the mediator at one or more wavelengths of light.

**20 Multiple Electrode Sensors and Calibration**

[0099] Multiple electrode sensors may be used for a variety of reasons. For example, multiple electrode sensors may be used to test a variety of analytes using a single sample. One embodiment of a multiple electrode sensor has one or more sample chambers which in turn may contain one or more working electrodes 22 with each working electrode 22 defining a different measurement zone. One or more of the working electrodes have the appropriate chemical reagents, for example, an appropriate enzyme, to test a first analyte and one or more of the remaining working electrodes have appropriate chemical reagents to test a second analyte. For example, a multiple electrode sensor might include 1) one or more working electrodes having glucose oxidase in the sensing layer to determine glucose concentration and 2) one or more working electrodes having lactate oxidase in the sensing layer to determine lactate concentration. Other combinations are also possible.

[0100] Multiple electrode sensors may also be used to improve the precision of the resulting readings. The measurements from each of the working electrodes (all of which are detecting the same analyte) can be averaged together to obtain a more precise reading. In some cases, measurements may be rejected if the difference between the value and the average exceeds a threshold limit. This threshold limit may be, for example, determined based on a statistical parameter, such as the standard deviation of the averaged measurements. The average may then be recalculated while omitting the rejected values. Furthermore, subsequent readings from an electrode that produced a rejected value may be ignored in later tests if it is assumed that the particular electrode is faulty. Alternatively, a particular electrode may be rejected only after having a predetermined number of readings rejected based on the readings from the other electrodes.

[0101] In addition to using multiple electrode sensors to increase precision, multiple measurements may be made at each electrode and averaged together to increase precision. This technique may also be used with a single electrode sensor to increase precision.

[0102] Errors in assays may occur when mass produced sensors are used because of variations in the volume of the measurement zone of the sensors. Two of the three dimensions of the measurement zone, the length and the width, are usually relatively large, between about 1-5 mm. Electrodes of such dimensions can be readily produced with a variance of 2% or less. The submicroliter measurement zone volume requires, however, that the third dimension be smaller than the length or width by one or two orders of magnitude. As mentioned hereinabove, the thickness of the sample chamber is typically between about 0.1 and about 0.01 mm. Manufacturing variances in the thickness may be as large or larger than the desired thickness. Therefore, it is desirable that a method be provided to accommodate for this uncertainty in the volume of sample within the measurement zone.

[0103] In one embodiment of the invention, depicted in Figure 5, multiple working electrodes 42, 44, 46 are provided on a base material 48. These electrodes are covered by another base, not shown, which has counter electrodes, not shown, disposed upon it to provide multiple facing electrode pairs. The variance in the separation distance between the working electrode and the counter electrode among the electrode pairs on a given sensor is significantly reduced, because the working electrodes and counter electrodes are each provided on a single base with the same spacer 28 between each electrode pair (see Figure 3).

[0104] One example of a multiple electrode sensor that can be used to accurately determine the volume of the measurement zones of the electrode pairs and also useful in reducing noise is presented herein. In this example, one

EP 0 958 495 B1

of the working electrodes 42 is prepared with a non-leachable redox mediator and a non-leachable second electron transfer agent (e.g., an enzyme). Sorbent material may be disposed between that working electrode 42 and its corresponding counter electrode. Another working electrode 44 includes non-leachable redox mediator, but no second electron transfer agent on the electrode. Again, this second electrode pair may have sorbent material between the working electrode 44 and the corresponding counter electrode. An optional third working electrode 46 has no redox mediator and no second electron transfer agent bound to the electrode, nor is there sorbent material between the working electrode 46 and its corresponding counter electrode.

[0105] The thickness of the sample chamber can be determined by measuring the capacitance, preferably in the absence of any fluid, between electrode 46 (or any of the other electrodes 42, 44 in the absence of sorbent material) and its corresponding counter electrode. The capacitance of an electrode pair depends on the surface area of the electrodes, the interelectrode spacing, and the dielectric constant of the material between the plates. The dielectric constant of air is unity which typically means that the capacitance of this electrode configuration is a few picofarads (or about 100 picofarads if there is fluid between the electrode and counter electrode given that the dielectric constant for most biological fluids is approximately 75). Thus, since the surface area of the electrodes are known, measurement of the capacitance of the electrode pair allows for the determination of the thickness of the measurement zone to within about 1-5%.

[0106] The amount of void volume in the sorbent material, can be determined by measuring the capacitance between electrode 44 (which has no second electron transfer agent) and its associated counter electrode, both before and after fluid is added. Upon adding fluid, the capacitance increases markedly since the fluid has a much larger dielectric constant. Measuring the capacitance both with and without fluid allows the determination of the spacing between the electrodes and the void volume in the sorbent, and thus the volume of the fluid in the reaction zone.

[0107] The sensor error caused by redox mediator in a non-uniform oxidation state prior to the introduction of the sample can be measured by concurrently electrolyzing the sample in the measurement zones that are proximate electrodes 42 and 44. At electrode 42, the analyte is electrolyzed to provide the sample signal. At electrode 44, the analyte is not electrolyzed because of the absence of the second electron transfer agent (assuming that a second electron transfer agent is necessary). However, a small charge will pass (and a small current will flow) due to the electrolysis of the redox mediator that was in a mixed oxidation state (i.e., some redox centers in the reduced state and some in the oxidized state) prior to the introduction of the sample. The small charge passed between the electrodes in this second electrode pair can be subtracted from the charge passed between the first electrode pair to substantially remove the error due to the oxidation state of the redox mediator. This procedure also reduces the error associated with other electrolyzed interferents, such as ascorbate, urate, and acetaminophen, as well as errors associated with capacitive charging and faradaic currents.

[0108] Other electrode configurations can also use these techniques (i.e., capacitance measurements and coulometric measurements in the absence of a critical component) to reduce background noise and error due to interferents and imprecise knowledge of the volume of the interrogated sample. Protocols involving one or more electrode pairs and one or more of the measurements described above can be developed and are within the scope of the invention. For example, only one electrode pair is needed for the capacitance measurements, however, additional electrode pairs may be used for convenience.

40 EXAMPLES

[0109] The invention will be further characterized by the following examples. These examples are not meant to limit the scope of the invention which has been fully set forth in the foregoing description. Variations within the concepts of the invention are apparent to those skilled in the art.

45 Example 1

**Preparation of a Small Volume *in vitro* Sensor for the Determination of Glucose Concentration**

[0110] A sensor was constructed corresponding to the embodiment of the invention depicted in Figure 1. The working electrode was constructed on a Mylar™ film (DuPont), the Mylar™ film having a thickness of 0.175 mm and a diameter of about 2.5 cm. An approximately 12 micron thick carbon pad having a diameter of about 1 cm was screen printed on the Mylar™ film. The carbon electrode was overlaid with a water-insoluble dielectric insulator (Insulayer) having a thickness of 12 µm, and a 4 mm diameter opening in the center.

[0111] The center of the carbon electrode, which was not covered by the dielectric, was coated with a redox mediator. The redox mediator was formed by complexing poly(1-vinyl imidazole) with Os(4,4'-dimethoxy-2,2'-bipyridine)<sub>2</sub>Cl<sub>2</sub> followed by cross-linking glucose oxidase with the osmium polymer using polyethylene glycol diglycidyl ether as described in Taylor, et al., *J. Electroanal. Chem.*, 396:511 (1995). The ratio of osmium to imidazole functionalities in the redox

EP 0 958 495 B1

mediator was approximately 1:15. The mediator was deposited on the working electrode in a layer having a thickness of 0.6  $\mu\text{m}$  and a diameter of 4 mm. The coverage of the mediator on the electrode was about 60  $\mu\text{g}/\text{cm}^2$  (dry weight). A spacer material was placed on the electrode surrounding the mediator-covered surface of the electrode. The spacer was made of poly(tetrafluoroethylene) (PTFE) and had a thickness of about 0.040 mm.

5 [0112] A sorbent material was placed in contact with the mediator-covered surface of the working electrode. The sorbent was made of nylon (Tetko Nitex nylon 3-10/2) and had a diameter of 5 mm, a thickness of 0.045 mm, and a void volume of about 20%. The volume of sample in the measurement zone was calculated from the dimensions and characteristics of the sorbent and the electrode. The measurement zone had a diameter of 4 mm (the diameter of the mediator covered surface of the electrode) and a thickness of 0.045 mm (thickness of the nylon sorbent) to give a volume of 0.57  $\mu\text{L}$ . Of this space, about 80% was filled with nylon and the other 20% was void space within the nylon sorbent. This resulting volume of sample within the measurement zone was about 0.11  $\mu\text{L}$ .

10 [0113] A counter/reference electrode was placed in contact with the spacer and the side of the sorbent opposite to the working electrode so that the two electrodes were facing each other. The counter/reference electrode was constructed on a Mylar<sup>TM</sup> film having a thickness of 0.175 mm and a diameter of about 2.5 cm onto which a 12 micron thick layer of silver/silver chloride having a diameter of about 1 cm was screen printed.

15 [0114] The electrodes, sorbent, and spacer were pressed together using plates on either side of the electrode assembly. The plates were formed of polycarbonate plastic and were securely clamped to keep the sensor together. The electrodes were stored in air for 48 hours prior to use.

20 [0115] Tabs extended from both the working electrode and the counter/reference electrode and provided for an electrical contact with the analyzing equipment. A potentiostat was used to apply a potential difference of +200mV between the working and counter/reference electrodes, with the working electrode being the anode. There was no current flow between the electrodes in the absence of sample, which was expected, as no conductive path between the electrodes was present.

25 [0116] The sample was introduced via a small tab of nylon sorbent material formed as an extension from the nylon sorbent in the sample chamber. Liquid was wicked into the sorbent when contact was made between the sample and the sorbent tab. As the sample chamber filled and the sample made contact with the electrodes, current flowed between the electrodes. When glucose molecules in the sample came in contact with the glucose oxidase on the working electrode, the glucose molecules were electrooxidized to gluconolactone. The osmium redox centers in the redox mediator then reoxidized the glucose oxidase. The osmium centers were in turn reoxidized by reaction with the working electrode. This provided a current which was measured and simultaneously integrated by a coulometer. (EG&G Princeton Applied Research Model #173)

30 [0117] The electrochemical reaction continued until the current reached a steady state value which indicated that greater than 95% of the glucose had been electroreduced. The current curve obtained by measurement of the current at specific intervals was integrated to determine the amount of charge passed during the electrochemical reaction. These charges were then plotted versus the known glucose concentration to produce a calibration curve.

35 [0118] The sensor was tested using 0.5  $\mu\text{L}$  aliquots of solutions containing known concentrations of glucose in a buffer of artificial cerebrospinal fluid or in a control serum (Baxter-Dade, Monitrol Level 1, Miami, FL) in the range of 3 to 20 mM glucose. The artificial cerebrospinal fluid was prepared as a mixture of the following salts: 126 mM NaCl, 27.5 mM NaHCO<sub>3</sub>, 2.4 mM KCl, 0.5 mM KH<sub>2</sub>PO<sub>4</sub>, 1.1 mM CaCl<sub>2</sub>·2H<sub>2</sub>O, and 0.5 mM Na<sub>2</sub>SO<sub>4</sub>.

40 [0119] The results of the analyses are shown in Table 1 and in Figure 7. In Table 1, Q<sub>avg</sub> is the average charge used to electrolyze the glucose in 3-6 identical test samples (Figure 7 graphs the charge for each of the test samples) and the 90% rise time corresponds to the amount of time required for 90% of the glucose to be electrolyzed. The data show a sensor precision of 10- 20%, indicating adequate sensitivity of the sensor for low glucose concentrations, as well as in the physiologically relevant range (30  $\mu\text{g}/\text{dL}$  - 600  $\mu\text{g}/\text{dL}$ ).

45

50

55

**TABLE 1**  
**Sensor Results Using Glucose Oxidase**

|                       | Number of Samples Tested | $Q_{avg}$ ( $\mu$ C) | 90% rise time (sec) |
|-----------------------|--------------------------|----------------------|---------------------|
| buffer only           | 4                        | $9.9 \pm 1.8$        | $13 \pm 6$          |
| 3 mM glucose/buffer   | 5                        | $17.8 \pm 3.5$       | $19 \pm 5$          |
| 6 mM glucose/buffer   | 4                        | $49.4 \pm 4.9$       | $25 \pm 3$          |
| 10 mM glucose/buffer  | 6                        | $96.1 \pm 12.4$      | $36 \pm 17$         |
| 15 mM glucose/buffer  | 5                        | $205.2 \pm 75.7$     | $56 \pm 23$         |
| 20 mM glucose/buffer  | 4                        | $255.7 \pm 41.0$     | $62 \pm 17$         |
| 4.2 mM glucose/serum  | 3                        | $44.2 \pm 4.3$       | $44 \pm 3$          |
| 15.8 mM glucose/serum | 3                        | $218.2 \pm 57.5$     | $72 \pm 21$         |

[0120] The average measured values of glucose concentration were fit by one or more equations to provide a calibration curve. Figure 8 shows the calibration curves for the glucose/buffer data of Table 1. One of the 15.0 mM glucose measurements was omitted from these calculations because it was more than two standard deviations away from the average of the measurements. The higher glucose concentrations (10-20 mM) were fit by a linear equation. The lower glucose concentrations were fit by a second order polynomial.

[0121] Figure 9 shows the data of Table 1 plotted on an error grid developed by Clarke, et al. *Diabetes Care*, 5, 622-27, 1987; for the determination of the outcome of errors based on inaccurate glucose concentration determination. The graph plots "true" glucose concentration vs. measured glucose concentration, where the measured glucose concentration is determined by calculating a glucose concentration using the calibration curves of figure 8 for each data point of figure 7. Points in zone A are accurate, those in zone B are clinically acceptable, and those in zones C, D, and E lead to increasingly inappropriate and finally dangerous treatments.

[0122] There were 34 data points. Of those data points 91% fell in zone A, 6% in zone B, and 3 % in zone C. Only one reading was determined to be in zone C. This reading was off-scale and is not shown in figure 9. Thus, 97% of the readings fell in the clinically acceptable zones A and B.

[0123] The total number of Os atoms was determined by reducing all of the Os and then electrooxidizing it with a glucose-free buffer in the sample chamber. This resulted in a charge of  $59.6 \pm 5.4 \mu$ C. Comparison of this result with the glucose-free buffer result in Table 1 indicated that less than 20% of the Os is in the reduced form prior to introduction of the sample. The variability in the quantity of osmium in the reduced state is less than 5% of the total quantity of osmium present.

#### Example 2

##### Response of the Glucose Sensor to Interferents

[0124] A sensor constructed in the same manner as described above for Example 1 was used to determine the sensor's response to interferents. The primary electrochemical interferents for blood glucose measurements are ascorbate, acetaminophen, and urate. The normal physiological or therapeutic (in the case of acetaminophen) concentration ranges of these common interferents are:

ascorbate: 0.034 - 0.114 mM

acetaminophen: 0.066 - 0.200 mM  
 urate (adult male): 0.27 - 0.47 mM

Tietz, in: *Textbook of Clinical Chemistry*, C.A. Burtis and E.R. Ashwood, eds., W.B. Saunders Co., Philadelphia 1994,  
 pp. 2210-12.

[0125] Buffered glucose-free interferent solutions were tested with concentrations of the interferents at the high end of the physiological or therapeutic ranges listed above. The injected sample volume in each case was 0.5  $\mu$ L. A potential of +100 mV or +200 mV was applied between the electrodes. The average charge ( $Q_{avg}$ ) was calculated by subtracting an average background current obtained from a buffer-only (i.e., interferent-free) solution from an average signal recorded with interferents present. The resulting average charge was compared with the signals from Table 1 for 4 mM and 10 mM glucose concentrations to determine the percent error that would result from the interferent.

**TABLE 2**  
**Interferent Response of Glucose Sensors**

| Solution             | E (mV) | n | $Q_{avg}$ ( $\mu$ C) | Error @ 4 mM glucose | Error @ 10 mM glucose |
|----------------------|--------|---|----------------------|----------------------|-----------------------|
| 0.114 mM ascorbate   | 100    | 4 | 0.4                  | 2%                   | <1%                   |
| 0.114 mM ascorbate   | 200    | 4 | -0.5                 | 2%                   | <1%                   |
| 0.2 mM acetaminophen | 100    | 4 | 0.1                  | <1%                  | <1%                   |
| 0.2 mM acetaminophen | 200    | 4 | 1.0                  | 5%                   | 1%                    |
| 0.47 mM urate        | 100    | 4 | 6.0                  | 30%                  | 7%                    |
| 0.47 mM urate        | 200    | 4 | 18.0                 | 90%                  | 21%                   |

[0126] These results indicated that ascorbate and acetaminophen were not significant interferents for the glucose sensor configuration, especially for low potential measurements. However, urate provided significant interference. This interference can be minimized by calibrating the sensor response to a urate concentration of 0.37 mM, e.g., by subtracting an appropriate amount of charge as determined by extrapolation from these results from all glucose measurements of the sensor. The resulting error due to a 0.10 mM variation in urate concentration (the range of urate concentration is 0.27 - 0.47 in an adult male) would be about 6% at 4 mM glucose and 100mV.

### Example 3

#### Sensor with Glucose Dehydrogenase

[0127] A sensor similar to that described for Example 1 was prepared and used for this example, except that glucose oxidase was replaced by pyrroloquinoline quinone glucose dehydrogenase and a potential of only +100 mV was applied as opposed to the +200 mV potential in Example 1. The results are presented in Table 3 below and graphed in Fig. 10.

**TABLE 3**  
**Sensor Results Using Glucose Dehydrogenase**

|                      | n | $Q_{avg}$ ( $\mu$ C) | 90% rise time (s) |
|----------------------|---|----------------------|-------------------|
| buffer               | 4 | 21.7 ± 5.2           | 14 ± 3            |
| 3 mM glucose/buffer  | 4 | 96.9 ± 15.0          | 24 ± 6            |
| 6 mM glucose/buffer  | 4 | 190.6 ± 18.4         | 26 ± 6            |
| 10 mM glucose/buffer | 4 | 327.8 ± 69.3         | 42 ± 9            |

[0128] The results indicated that the charge obtained from the glucose dehydrogenase sensor was much larger than for the comparable glucose oxidase sensor, especially for low concentrations of glucose. For 4 mM glucose concentrations the measurements obtained by the two sensors differed by a factor of five. In addition, the glucose dehydrogenase sensor operated at a lower potential, thereby reducing the effects of interferent reactions.

[0129] In addition, the results from Table 3 were all fit by a linear calibration curve as opposed to the results in Example 1, as shown in Fig. 10. A single linear calibration curve is greatly preferred to simplify sensor construction and operation.

[0130] Also, assuming that the interferent results from Table 2 are applicable for this sensor, all of the interferents would introduce an error of less than 7% for a 3 mM glucose solution at a potential of 100 mV.

#### Example 4

##### Determination of Lactate Concentration in a Fluid Stream

[0131] The sensor of this Example was constructed using a flow cell (BioAnalytical Systems, Inc. # MF-1025) with a glassy carbon electrode. A redox mediator was coated on the electrode of the flow cell to provide a working electrode. In this case, the redox mediator was a polymer formed by complexing poly(1-vinyl imidazole) with Os(4,4'-dimethyl-2,2'-bipyridine)<sub>2</sub>Cl<sub>2</sub> with a ratio of 1 osmium for every 15 imidazole functionalities. Lactate oxidase was cross-linked with the polymer via polyethylene glycol diglycidyl ether. The mediator was coated onto the electrode with a coverage of 500  $\mu$ g/cm<sup>2</sup> and a thickness of 5  $\mu$ m. The mediator was covered by a polycarbonate track-etched membrane (Osmonics-Poretics #10550) to improve adherence in the flow stream. The membrane was then overlaid by a single 50  $\mu$ m thick spacer gasket (BioAnalytical Systems, Inc. #MF-1062) containing a void which defined the sample chamber and corresponding measurement zone. Assembly of the sensor was completed by attachment of a cell block (BioAnalytical Systems, Inc. #MF-1005) containing the reference and auxiliary electrodes of the flow cell.

[0132] The sample chamber in this case corresponded to a 50  $\mu$ m thick cylinder (the thickness of the spacer gasket) in contact with a mediator-coated electrode having a surface area of 0.031 cm<sup>2</sup>. The calculated volume of sample in the measurement zone of this sensor was approximately 0.16  $\mu$ L.

[0133] The flow rate of the fluid stream was 5  $\mu$ L/min. A standard three electrode potentiostat was attached to the cell leads and a potential of +200 mV was applied between the redox mediator-coated glassy carbon electrode and the reference electrode. This potential was sufficient to drive the enzyme-mediated oxidation of lactate.

[0134] As the fluid stream flowed through the sensor, a steady-state current proportional to the lactate concentration was measured. At periodic intervals the fluid flow was stopped and current was allowed to flow between the electrodes until approximately all of the lactate in the measurement zone was electrooxidized, as indicated by the achievement of a stabilized, steady-state current. The total charge, Q, required for lactate electrooxidation was found by integration of the differential current registered from the flow stoppage until the current reached a steady-state. The concentration was then calculated by the following equation:

$$[\text{lactate}] = Q/2FV \quad (4)$$

where V is the volume of sample within the measurement zone and F is Faraday's constant.

[0135] This assay was performed using lactate solutions having nominal lactate concentrations of 1.0, 5.0, and 10.0 mM. The measured concentrations for the assay were 1.9, 5.4, and 8.9 mM respectively.

#### Example 5

##### 5 Determination of the Oxidation State of Os(4,4'-dimethoxy-2,2'-bipyridine)<sub>2</sub>Cl<sup>+/+2</sup> Complexed with poly(1-vinyl imidazole)

[0136] A sensor having a three electrode design was commercially obtained from Ecossensors Ltd., Long Hanborough, England, under the model name "large area disposable electrode". The sensor contained parallel and coplanar working, reference and counter electrodes. The working surface area (0.2 cm<sup>2</sup>) and counter electrodes were formed of printed carbon and the reference electrode was formed of printed Ag/AgCl. A redox mediator was coated on the carbon working electrode. The redox mediator was formed by complexation of poly(1-vinyl imidazole) with Os(4,4'-dimethoxy-2,2'-bipyridine)<sub>2</sub>Cl<sub>2</sub> in a ratio of 15 imidazole groups per Os cation followed by cross linking the osmium polymer with glucose oxidase using polyethylene glycol diglycidyl ether.

[0137] The electrode was cured at room temperature for 24 hours. The coplanar electrode array was then immersed in a buffered electrolyte solution, and a potential of +200 mV (sufficient for conversion of Os(II) to Os(III),) was applied between the working electrode and the reference electrode.

[0138] Upon application of the potential, an undetectable charge of less than 1 µC was passed. Subsequent reduction and reoxidation of the redox mediator yielded a charge for conversion of all Os from Os(II) to Os(III) of 65 µC. Therefore, more than 98% of the Os cations in the redox mediator were in the desired oxidized Os(III) state.

#### Example 6

##### 25 Determination of the Oxidation State of the Os(4,4'-dimethoxy-2,2'-bipyridine)<sub>2</sub>Cl<sup>+/+2</sup> Complexed with poly (4-vinyl pyridine)

[0139] A similar experiment to that of Example 5 was conducted with the same working/counter/reference electrode configuration except that the redox mediator on the working electrode was changed to a complex of Os(4,4'-dimethoxy-2,2'-bipyridine)<sub>2</sub>Cl<sub>2</sub> with poly(4-vinyl pyridine), with 12 pyridine groups per Os cation, cross linked with glucose oxidase via polyethylene glycol diglycidyl ether.

[0140] Two sensors were constructed. The electrodes of the two sensors were cured at room temperature for 24 hours. The electrodes were then immersed in a buffered electrolyte solution and a potential of +200 mV was applied between the working and reference electrodes.

[0141] Upon application of the potential to the electrodes, a charge of 2.5 µC and 3.8 µC was passed in the two sensors, respectively. Subsequent reduction and reoxidation of the redox mediators yielded oxidation charges of 27.9 µC and 28.0 µC, respectively. Therefore, the sensors originally contained 91% and 86% of the Os cations in the desirable oxidized Os(III) state.

#### 40 Example 7

##### Optical Sensor

[0142] An optical sensor is constructed by applying a film of redox polymer with crosslinked enzyme onto a light-transparent support such as a glass slide. The quantity of redox mediator is equal to or greater than (in a stoichiometric sense) the maximum quantity of analyte expected to fill the measurement zone. The spacer material, sorbent and facing support are securely clamped. The sample chamber is adapted to transmit light through the assembled sensor to an optical density detector or to a fluorescence detector. As sample fills the sample chamber and the redox mediator is oxidized, changes in the absorption, transmission, reflection or fluorescence of the redox mediator in the chamber are correlated to the amount of glucose in the sample.

#### Example 8

##### Blood Volumes from Upper Arm Lancet Sticks

[0143] The forearm of a single individual was pierced with a lancet multiple times in order to determine the reproducibility of blood volumes obtained by this method. Despite more than thirty lancet sticks in the anterior portion of each forearm and the dorsal region of the left forearm, the individual identified each stick as virtually painless.

[0144] The forearm was pierced with a Payless Color Lancet. The blood from each stick was collected using a 1  $\mu\text{L}$  capillary tube, and the volume was determined by measuring the length of the blood column. The volumes obtained from each stick are shown below in Table 4.

Table 4

| Volume of Lancet Sticks |                             |                              |                           |
|-------------------------|-----------------------------|------------------------------|---------------------------|
|                         | Left Anterior Forearm, (nL) | Right Anterior Forearm, (nL) | Left Dorsal Forearm, (nL) |
| 1                       | 180                         | 190                          | 180                       |
| 2                       | 250                         | 180                          | 300                       |
| 3                       | 170                         | 120                          | 310                       |
| 4                       | 150                         | 100                          | 300                       |
| 5                       | 100                         | 210                          | 60                        |
| 6                       | 50                          | 140                          | 380                       |
| 7                       | 90                          | 120                          | 220                       |
| 8                       | 130                         | 140                          | 200                       |
| 9                       | 120                         | 100                          | 380                       |
| 10                      |                             | 100                          | 320                       |
| 11                      |                             |                              | 260                       |
| 12                      |                             |                              | 250                       |
| 13                      |                             |                              | 280                       |
| 14                      |                             |                              | 260                       |
| Avg.                    | 138 $\pm$ 58 nL             | 140 $\pm$ 40 nL              | 264 $\pm$ 83 nL           |

[0145] The invention has been described with reference to various specific and preferred embodiments and techniques. However, it will be apparent to one of ordinary skill in the art that many variations and modifications may be made while remaining within the scope of the invention.

### Claims

1. An electrochemical sensor for determining the concentration of an analyte in a sample, the sensor comprising;
  - 40 at least one working electrode (22);
  - at least one counter electrode (24);
  - which electrodes, in use, are connected to external electronics of a measuring device;
  - at least one sample chamber (26), wherein the at least one sample chamber is
    - 45 (i) a sample chamber for holding the sample in electrolytic contact with the working electrode and sized to contain no more than about 1  $\mu\text{l}$  of sample; or
    - (ii) a sample chamber comprising at least one measurement zone sized to contain no more than about 1  $\mu\text{l}$  of sample, wherein the measurement zone is bounded on at least two sides by the working and counter electrodes;
  - 50 said sensor containing a non-leachable redox mediator on the working electrode;
  - and
  - said sensor optionally containing a sorbent material (34) disposed at least partially within the sample chamber or at least partially within the measurement zone.
- 55 2. The sensor of claim 1, wherein the working electrode and the counter electrode comprise metal or carbon, and the sensor includes the non-leachable redox mediator on the working electrode.

3. The sensor of claim 2, wherein the sensor further comprises a second electron transfer agent, preferably an enzyme such as glucose oxidase, on the working electrode, wherein the second transfer agent is optionally immobilized on the working electrode and/or is optionally non-leachable.
5. The sensor of claim 1, wherein the working electrode and the counter electrode comprise metal or carbon, and the sensor includes the sorbent material disposed at least partially within the sample chamber or at least partially within the measurement zone.
10. The sensor of any of claims 1 through 4, wherein the sample chamber or, the measurement zone, is sized to contain no more than about 0.5  $\mu$ L, preferably no more than about 0.2  $\mu$ L, preferably no more than about 0.1  $\mu$ L of sample.
15. The sensor of any of claims 1 through 5, wherein the redox mediator is immobilized on the working electrode.
20. The sensor of any of claims 1 through 6, wherein the redox mediator is an air-oxidizable redox mediator, preferably with at least 90% of the air-oxidizable redox mediator in an oxidized state prior to introduction of sample.
25. The sensor of any of claims 1 through 7, wherein the redox mediator comprises a transition metal complex, such as an osmium, ruthenium, iron, or cobalt complex; and preferably is osmium complexed with at least one ligand having a nitrogen-containing heterocycle, such as 2,2'-bipyridine, 4,4'-dimethyl-2,2'-bipyridine, 4,4'-dialkoxy-2,2'-bipyridine, 1,10-phenanthroline, 4,7-dimethyl-1,10-phenanthroline, 4,7-dialkoxy-1,10-phenanthroline, or derivatives thereof.
30. The sensor of claim 8, wherein the ligand having a nitrogen-containing heterocycle comprises 2,2'-bipyridine, 1,10-phenanthroline, or a derivative thereof; such as a mono-, di-, or polyalkoxy derivative of 2,2'-bipyridine or 1,10-phenanthroline, wherein the carbon to oxygen ratio of the alkoxy functional groups is sufficient to retain solubility of the transition metal complex in water prior to crosslinking.
35. The sensor of claim 8 or 9, wherein the carbon to oxygen ratio of the alkoxy functional groups is sufficient to retain solubility of the transition metal complex in water prior to crosslinking.
40. The sensor of any of claims 1 through 10, wherein the sorbent material has a void volume of about 5% to 50%, preferably about 10% to 25%, of the total volume of the sorbent material.
45. The sensor of any of claims 1 through 11, wherein the sensor further comprises one or more additional working electrodes.
50. The sensor of any of claims 1 through 12, wherein at least one working electrode and at least one counter electrode form at least one facing electrode pair, optionally wherein each pair is responsive to a specific analyte.
55. The sensor of claim 13, wherein the working electrode and counter electrode have a separation distance of no more than about 0.2 mm, or no more than about 0.1 mm, or no more than about 0.05 mm.
18. The sensor of claim 13, wherein at least one facing electrode pair comprises a working electrode including non-leachable enzyme and redox mediator, and wherein at least one other facing electrode pair comprises a working electrode including non-leachable redox mediator in the absence of the enzyme.
17. The sensor of any of claims 1 through 16, wherein the working electrode comprises a first arm (122) and the counter electrode comprises a second arm (124), a portion of the first arm overlapping a portion of the second arm, wherein the measurement zone or, the sample chamber, comprises a region (21) between the overlapping portions of the first and second arms.
16. The sensor of claim 15, further comprising a third electrode (46) pair having no redox mediator or enzyme on the working electrode.
19. The sensor of any of claims 1 through 18, wherein the first arm has an extra length and the overlapping portion of the first arm has a width, wherein a ratio of the extra length of the first arm to the width of the overlapping portion of the first arm ranges from 0.1:1 to 50:1, preferably from 1:1 to 15:1, and more preferably from 4:1 to 10:1.

19. The sensor of claim 18, wherein the first and second arms intersect at an angle greater than 0 degrees.
20. The sensor of any of claims 1 through 19, wherein the sorbent material comprises a powdered material disposed on the working electrode.  
5
21. The sensor of claim 13, wherein the at least one facing electrode pair comprises a base material (102) having a recess (104) and at least one of the working electrode and the counter electrode disposed in the recess.
22. The sensor of any of claims 1 through 21, further comprising a filler material, preferably a hydrophilic filler material, wherein the filler material is disposed in the measurement zone or in the sample chamber, to decrease a volume of the measurement zone or the sample chamber available for the sample.  
10
23. The sensor of claims 1 through 22, wherein the sensor produces a signal in a buffer solution containing 10 mM glucose that is at least 9 times greater than a signal produced in a buffer solution with no glucose.  
15
24. A method for determining a concentration of an analyte in a sample, comprising contacting the sample with the electrochemical sensor of any of claims 1 through 23, and determining the concentration of the analyte in the sample by coulometry.
25. The method of claim 24, wherein the contacting step is performed by contacting the sample with the sorbent material to wick the sample into the sample chamber or the measurement zone.  
20
26. The method of claim 24, wherein the sample chamber fills by capillary action.
27. The method of claim 24, wherein the step of determining the concentration of the analyte comprises:  
30  
electrolyzing at least 90% of analyte present in the measurement zone by applying a potential across the working and counter electrodes, preferably in less than about 5 minutes, and more preferably in less than about 1 minute;  
determining an electrical charge used to electrolyze the analyte; and  
correlating the electrical charge with the concentration of the analyte in the sample;  
wherein the determining step is optionally performed by the following steps:  
measuring a current generated at the working electrode at two or more times as the analyte is electrolyzed;  
35  
and  
integrating the measured currents over time to obtain the electrical charge used to electrolyze the analyte.
28. The method of claim 24, wherein the step of determining the concentration of the analyte by coulometry comprises the steps of:  
40  
electrolyzing a portion of the analyte by applying a potential across the working and the counter electrode;  
measuring a current generated at the working electrode at two or more times during the electrolysis;  
extrapolating a current curve based on the measured currents;  
integrating the current curve over time to obtain an electrical charge necessary to electrolyze at least 90% of  
45  
the analyte; and  
correlating the electrical charge with the concentration of the analyte in the sample.
29. The method of claim 24 wherein the electrochemical sensor comprises first and second electrode pairs, each pair comprising a working electrode, wherein said first electrode pair includes a non-leachable redox mediator and a non-leachable enzyme on the working electrode, and wherein said second electrode pair includes non-leachable redox mediator on the working electrode in the absence of enzyme.  
50
30. The method of claim 29, wherein the step of determining the concentration of analyte comprises the steps of:  
55  
measuring substantially simultaneously, and at two or more times, a first current generated at the first electrode pair and a second current generated at the second electrode pair;  
Integrating the measured first currents over time to obtain a first charge;  
integrating the measured second currents over time to obtain a second charge;

subtracting the second charge from the first charge to obtain a noise-reduced charge; and correlating the concentration of the analyte to the noise-reduced charge.

31. The method of claim 24, the method comprising, prior to the contacting and determining steps, the further steps of:

5 providing the electrochemical sensor of any of claims 1 through 23, wherein the sensor has one or more facing electrode pairs, each electrode pair comprising a working electrode, a counter electrode, and a measurement zone between the working electrode and the counter electrode;

10 measuring a capacitance of at least one of the electrode pairs; and calculating the volume of the measurement zone from the capacitance measurement.

32. The method of claim 24, wherein the sensor includes a redox mediator on the working electrode, and the molar amount of redox mediator in a reduced form prior to introduction of the sample is less than, on a stoichiometric basis, 5% of the expected molar amount of the analyte to be electrolyzed; and wherein the step of determining the concentration of analyte comprises

15 electrolyzing less than about 1  $\mu\text{L}$  of sample.

33. The method of claim 32, wherein the sensor comprises at least two working electrodes, each working electrode having an associated measurement zone, and wherein the step of determining the concentration of the analyte comprises averaging measurements from the at least two working electrodes, and optionally further comprises eliminating measurements which exceed a threshold value, and optionally further comprises reaveraging the measurements without the eliminated measurements.

- 20 34. An analyte measurement system comprising:

25 sample acquisition means, preferably a skin-piercing member (54), such as a lancet, for producing a patient sample;

the electrochemical sensor of any one of claims 1 through 23; and

30 optionally a transport means, such as a wicking material, a capillary chamber, a sorbent material or a pump, for transporting the sample produced by the sample acquisition means to the sample chamber or the measurement zone.

- 35 35. The system of claim 34 wherein the skin piercing member is integral with the sensor.

36. A method for measuring analyte in a patient sample, the method comprising:

contacting the patient with an analyte measuring system, the system comprising:

40 sample acquisition means for producing a patient sample; and the electrochemical sensor of any of claims 1 through 23, for measuring analyte in the sample;

45 acquiring a sample using the sample acquisition means;

transporting a portion of the sample to the measurement zone or sample chamber of the electrochemical sensor, wherein the transporting step optionally comprising wicking the sample into the measurement zone or sampler chamber using the sorbent material; and determining the concentration of the analyte in the sample by coulometry.

37. The method of claim 36, which the sample acquisition means is integral with the sensor.

50 38. The method of claims 36 or 37, wherein the sample acquisition means comprises a skin-piercing member, such as a lancet, and the step of acquiring a sample comprises piercing the patient's skin at a location other than at a finger of the patient to produce a sample.

39. A method of determining a concentration of an analyte in a sample, the method comprising steps of:

55 connecting the electrodes of an electrochemical sensor comprising a working electrode, a counter electrode, and a sample chamber for holding the sample in electrolytic contact with the working electrode and counter electrode, to external electronics of a measuring device;

- contacting the sample with the sensor;  
holding the sample within the sample chamber in a non-flowing manner;  
applying a potential between the working and counter electrodes to electrolyze the analyte in a portion of the sample within the sample chamber, wherein the portion of the sample in which the analyte is electrolyzed has  
5 a volume of less than 1  $\mu$ L;  
measuring current generated by the electrochemical sensor at a plurality of times while the analyte in the portion of the sample is being electrolyzed; and  
determining, by coulometry, a concentration of the analyte in the sample using the measured currents.
- 10 40. The sensor of claim 7, wherein the sensor further comprises a second electron transfer agent, such as an enzyme, coated on the support and in contact with the redox mediator, wherein the second electron transfer agent is optionally immobilized on the support.
- 15 41. A method for determining a concentration of an analyte in a sample, comprising the steps of:  
contacting the sample with the sensor of claim 7 or claim 40; and  
correlating the concentration of the analyte in the sample to a change in oxidation state of the redox mediator in the presence of analyte.
- 20 42. The method of claim 41, wherein the sensor comprises an optical sensor, and the step of correlating the concentration of the analyte comprises:  
irradiating the redox mediator with light;  
measuring the response of the redox mediator to irradiation by light; and  
25 correlating the concentration of the analyte to the measured response of the redox mediator.
43. The method of claim 42, wherein the step of measuring the response of the redox mediator to irradiation by light comprises measuring the absorption, or the transmittance, of the irradiated light by the redox mediator.
- 30 44. The method of claim 42, wherein the step of measuring the response of the redox mediator to irradiation by light comprises measuring the fluorescence of the redox mediator after irradiation by light, or measuring the reflection of light by the redox mediator.
45. The method of claim 41, wherein the sensor comprising an electrochemical sensor, and the step of correlating the concentration of the analyte comprises:  
35 applying an electrical potential across the redox mediator;  
measuring a current at one or more intervals, the current being generated in response to the electrolysis of the redox mediator in the presence of the analyte; and  
40 correlating the concentration of the analyte to the measured current.
46. The method of claim 41, wherein the redox mediator comprises a transition metal complex, such as an osmium complex, and preferably, osmium complexed with at least one ligand having a nitrogen-containing heterocycle, such as 2,2'-bipyridine, 1,10-phenanthroline, or a derivative thereof, preferably a mono-, di-, or polyalkoxy derivative of 2,2'-bipyridine or 1,10-phenanthroline, and more preferably comprises 4,4'-dialkoxy-2,2'-bipyridine or 4,7-dialkoxy-1,10-phenanthroline, wherein the carbon to oxygen ratio of the alkoxy functional groups is sufficient to retain solubility of the transition metal complex in water prior to crosslinking.  
45
47. The method of claim 46, wherein the nitrogen-containing heterocycle comprises 4,4'-dimethoxy-2,2'-bipyridine or 4,7-dimethoxy-1,10-phenanthroline.  
50
48. The method of claim 46, wherein the osmium complex comprises osmium complexed with a polymeric ligand, wherein the polymeric ligand comprises a nitrogen-containing heterocycle.
- 55 49. The method of claim 48, wherein the polymer comprises poly(4-vinyl pyridine) or poly (1-vinyl imidazole).
50. The method of claim 49, wherein the redox mediator comprises Os[4,4'-dimethoxy-2,2'-bipyridine]<sub>2</sub>Cl<sup>+/+2</sup> or Os [4,7-dimethoxy-1,10-phenanthroline]<sub>2</sub>Cl<sup>+/+2</sup> complexed with poly(1-vinyl imidazole).

51. The sensor of claim 7, wherein a portion of the air-oxidizable redox mediator is oxidized when packaging the analytical sensor in an atmosphere containing molecular oxygen.
52. The method of claim 50, wherein greater than 90% of the redox mediator is in an oxidized state after being stored for more than one month.
53. An analyte measurement system comprising:
  - 10 a. a sensor of any of the claims 1-23, 40, and 51; and
  - b. a coulometer operatively connected to the sensor and configured to measure the cumulative electrical charge flowing through the sensor.

**Patentansprüche**

- 15 1. Elektrochemischer Sensor zur Bestimmung der Konzentration eines Analyten in einer Probe, wobei der Sensor aufweist:
  - 20 wenigstens eine Arbeitselektrode (22);
  - wobei die Elektroden, im Gebrauch, mit einer externen Elektronik einer Meßvorrichtung verbunden sind;
  - 25 wenigstens eine Probenkammer (26), wobei die wenigstens eine Probenkammer  
(i) eine Probenkammer ist, die die Probe in elektrolytischem Kontakt mit der Arbeitselektrode hält und so bemessen ist, daß sie nicht mehr als etwa 1 µl der Probe enthält; oder  
(ii) eine Probenkammer ist, die wenigstens eine Meßzone aufweist, die so bemessen ist, daß sie nicht mehr als etwa 1 µl Probe enthält, wobei die Meßzone auf wenigstens zwei Seiten von der Arbeits- und der Gegen-elektrode begrenzt ist;
  - 30 wobei der Sensor einen nicht auslaugbaren Redoxmediator auf der Arbeitselektrode enthält; und  
wobei der Sensor gegebenenfalls ein Sorbensmaterial (34) enthält, das wenigstens teilweise innerhalb der Probenkammer oder wenigstens teilweise innerhalb der Meßzone angeordnet ist.
  - 35 2. Sensor nach Anspruch 1, bei dem die Arbeitselektrode und die Gegen-elektrode Metall oder Kohlenstoff umfassen, und der Sensor den nicht auslaugbaren Redoxmediator auf der Arbeitselektrode enthält.
  - 40 3. Sensor nach Anspruch 2, wobei der Sensor außerdem ein zweites Elektronenübertragungsmittel, vorzugsweise ein Enzym, wie beispielsweise Glucoseoxidase, auf der Arbeitselektrode aufweist, wobei das zweite Übertragungs-mittel gegebenenfalls auf der Arbeitselektrode immobilisiert ist und/oder gegebenenfalls nicht auslaugbar ist.
  - 45 4. Sensor nach Anspruch 1, wobei die Arbeitselektrode und die Gegen-elektrode Metall oder Kohlenstoff umfassen, und der Sensor das Sorbensmaterial einschließt, das wenigstens teilweise innerhalb der Probenkammer oder wenigstens teilweise innerhalb der Meßzone angeordnet ist.
  5. Sensor nach irgendeinem der Ansprüche 1 bis 4, wobei die Probenkammer oder die Meßzone so bemessen ist, daß sie nicht mehr als etwa 0,5 µl, vorzugsweise nicht mehr als etwa 0,2 µl, vorzugsweise nicht mehr als etwa 0,1 µl der Probe enthält.
  - 50 6. Sensor nach irgendeinem der Ansprüche 1 bis 5, wobei der Redoxmediator auf der Arbeitselektrode immobilisiert ist.
  7. Sensor nach irgendeinem der Ansprüche 1 bis 6, wobei der Redoxmediator ein luftoxidierbarer Redoxmediator ist, wobei vorzugsweise wenigstens 90% des luftoxidierbaren Redoxmediators vor der Einführung der Probe in einem oxidierten Zustand vorliegt.
  - 55 8. Sensor nach irgendeinem der Ansprüche 1 bis 7, wobei der Redoxmediator einen Übergangsmetallkomplex um-faßt, wie beispielsweise einen Osmium-, Ruthenium-, Eisen- oder Cobaltkomplex, und vorzugsweise Osmium ist,

**EP 0 958 495 B1**

das mit wenigstens einem Liganden mit einem stickstoffhaltigen Heterocyclus komplexiert ist, wie beispielsweise mit 2,2'-Bipyridin, 4,4'-Dimethyl-2,2'-bipyridin, 4,4'-Dialkoxy-2,2'-bipyridin, 1,10-Phenanthrolin, 4,7-Dimethyl-1,10-phenanthrolin, 4,7-Dialkoxy-1,10-phenanthrolin oder Derivaten davon.

- 5 9. Sensor nach Anspruch 8, wobei der Ligand mit einem stickstoffhaltigen Heterocyclus 2,2'-Bipyridin, 1,10-phenanthrolin oder ein Derivat davon umfaßt, wie beispielsweise ein Mono-, Di- oder Polyalkoxyderivat von 2,2'-Bipyridin oder 1,10-Phenanthrolin, wobei das Verhältnis von Kohlenstoff zu Sauerstoff der funktionellen Alkoxygruppe ausreicht, die Löslichkeit des Übergangsmetallkomplexes in Wasser vor dem Vernetzen zu gewährleisten.
- 10 10. Sensor nach Anspruch 8 oder 9, wobei das Verhältnis von Kohlenstoff zu Sauerstoff der funktionellen Alkoxygruppen ausreicht, die Löslichkeit des Übergangsmetallkomplexes in Wasser vor dem Vernetzen zu gewährleisten.
- 15 11. Sensor nach irgendeinem der Ansprüche 1 bis 10, wobei das Sorbensmaterial ein freies Volumen von etwa 5% bis 50%, vorzugsweise von etwa 10% bis 25% des Gesamtvolumens des Sorbensmaterials aufweist.
12. Sensor nach irgendeinem der Ansprüche 1 bis 11, wobei der Sensor außerdem eine oder mehrere zusätzliche Arbeitselektroden aufweist.
- 20 13. Sensor nach irgendeinem der Ansprüche 1 bis 12, wobei wenigstens eine Arbeitselektrode und wenigstens eine Gegenelektrode wenigstens einander gegenüberliegendes Elektrodenpaar bilden, wobei gegebenenfalls jedes Paar auf einen spezifischen Analyten anspricht.
- 25 14. Sensor nach Anspruch 13, wobei die Arbeitselektrode und die Gegenelektrode durch einen Abstand von nicht mehr als etwa 0,2 mm, oder nicht mehr als etwa 0,1 mm, oder nicht mehr als etwa 0,05 mm voneinander getrennt sind.
- 30 15. Sensor nach Anspruch 13, wobei wenigstens ein Paar sich gegenüberliegender Elektroden eine Arbeitselektrode umfaßt, die ein nicht auslaugbares Enzym und einen Redoxmediator aufweist, und worin wenigstens ein anderes Paar von sich gegenüberliegenden Elektroden eine Arbeitselektrode umfaßt, die einen nicht auslaugbaren Redoxmediator in Abwesenheit des Enzyms enthält.
16. Sensor nach Anspruch 15, der außerdem ein drittes Elektrodenpaar (46) aufweist, bei dem auf der Arbeitselektrode kein Redoxmediator oder Enzym vorhanden ist.
- 35 17. Sensor nach irgendeinem der Ansprüche 1 bis 16, wobei die Arbeitselektrode einen ersten Arm (122) und die Gegenelektrode einen zweiten Arm (124) aufweisen, wobei ein Teil des ersten Arms einen Abschnitt des zweiten Arms überlappt, wobei die Meßzone oder die Probenkammer einen Bereich (21) zwischen den überlappenden Abschnitten des ersten Arms und des zweiten Arms umfassen.
- 40 18. Sensor nach Anspruch 17, wobei der erste Arm eine Extralänge aufweist und der überlappende Abschnitt des ersten Arms eine Breite aufweist, wobei ein Verhältnis der Extralänge des ersten Arms zu der Breite des überlappenden Abschnitts des ersten Arms im Bereich von 0,1:1 zu 50:1, vorzugsweise von 1:1 bis 15:1 und besonders bevorzugt von 4:1 bis 10:1 beträgt.
- 45 19. Sensor nach Anspruch 18, wobei die ersten und zweiten Arme sich unter einem Winkel von mehr als 0 Grad überschneiden.
20. Sensor nach irgendeinem der Ansprüche 1 bis 19, wobei das Sorbensmaterial ein pulverförmiges Material umfaßt, das auf der Arbeitselektrode angeordnet ist.
- 50 21. Sensor nach Anspruch 13, wobei das wenigstens eine Paar sich gegenüberliegender Elektroden ein Basismaterial (102) mit einer Ausnehmung (104) umfaßt und wenigstens eine von der Arbeitselektrode und der Gegenelektrode in der Ausnehmung angeordnet ist.
- 55 22. Sensor nach irgendeinem der Ansprüche 1 bis 21, der außerdem ein Füllstoffmaterial aufweist, vorzugsweise ein hydrophiles Füllstoffmaterial, wobei das Füllstoffmaterial in der Meßzone oder in der Probenkammer angeordnet ist, um ein Volumen der Meßzone oder der Probenkammer zu verringern, das für die Probe zur Verfügung steht.

**EP 0 958 495 B1**

23. Sensor nach den Ansprüchen 1 bis 22, wobei der Sensor in einer Pufferlösung, die 10 mM Glucose enthält, ein Signal erzeugt, das wenigstens 9 mal größer ist als ein Signal, das in einer Pufferlösung ohne Glucose erzeugt wird.
- 5 24. Verfahren zur Bestimmung einer Konzentration eines Analyten in einer Probe, das das Inkontaktbringen der Probe mit dem elektrochemischen Sensor nach irgendeinem der Ansprüche 1 bis 23 und die Bestimmung der Konzentration des Analyten in der Probe mittels Coulometrie umfaßt.
- 10 25. Verfahren nach Anspruch 24, wobei die Stufe des Inkontaktbringens dadurch durchgeführt wird, daß man die Probe mit dem Sorbensmaterial in Kontakt bringt, um die Probe in die Probenkammer oder Meßzone einzusaugen.
- 15 26. Verfahren nach Anspruch 24, wobei die Probenkammer durch Kapillarwirkung gefüllt wird.
- 20 27. Verfahren nach Anspruch 24, wobei der Schritt der Bestimmung der Konzentration des Analyten umfaßt:
  - 15 Elektrolysieren von wenigstens 90% des Analyten, der in einer Meßzone vorhanden ist, dadurch, daß man ein Potential zwischen der Arbeits- und der Gegenelektrode anlegt, und zwar vorzugsweise in weniger als etwa 5 Minuten, und stärker bevorzugt in weniger als etwa 1 Minute;
  - 25 Bestimmen einer elektrischen Ladung, die zur Elektrolyse des Analyten gebraucht wird; und Korrelieren der elektrischen Ladung mit der Konzentration des Analyten in der Probe,
- 20 wobei die Bestimmungsstufe gegebenenfalls mit den folgenden Stufen durchgeführt wird:
  - 25 Messen eines Stroms, der an der Arbeitselektrode erzeugt wird, zu zwei oder mehr Zeitpunkten, während der Analyt elektrolysiert wird; und
  - 30 Integrieren der gemessenen Ströme über die Zeit, um die elektrische Ladung zu erhalten, die für die Elektrolyse des Analyten gebraucht wird.
- 35 28. Verfahren nach Anspruch 24, wobei die Stufe der Bestimmung der Konzentration des Analyten durch Coulometrie die Schritte umfaßt:
  - 30 Elektrolysieren eines Teils eines Analyten dadurch, daß man ein Potential an die Arbeitselektrode und Gegenelektrode anlegt;
  - 35 Messen eines Stroms, der an der Arbeitselektrode erzeugt wird, zu zwei oder mehr Zeitpunkten während der Elektrolyse;
  - 40 Extrapolieren einer Stromkurve auf der Basis der gemessenen Ströme;
  - 45 Integrieren der Stromkurve über die Zeit, um eine elektrische Ladung zu erhalten, die erforderlich ist, um wenigstens 90% des Analyten zu elektrolysiern; und
  - 50 Korrelieren der elektrischen Ladung mit der Konzentration des Analyten in der Probe.
- 45 29. Verfahren nach Anspruch 24, wobei der elektrochemische Sensor erste und zweite Elektrodenpaare aufweist, wobei jedes Paar eine Arbeitselektrode umfaßt, wobei das erste der Elektrodenpaare einen nicht auslaugbaren Redoxmediator und ein nicht auslaugbares Enzym auf der Arbeitselektrode aufweist, und wobei das zweite der Elektrodenpaare einen nicht auslaugbaren Redoxmediator in Abwesenheit von Enzym auf der Arbeitselektrode aufweist.
- 50 30. Verfahren nach Anspruch 29, wobei die Stufe der Bestimmung der Konzentration des Analyten die Schritte umfaßt:
  - 50 im wesentlichen gleichzeitig, und zu zwei oder mehr Zeitpunkten, Messen eines ersten Stroms, der an dem ersten Elektrodenpaar erzeugt wird, sowie eines zweiten Stroms, der an dem zweiten Elektrodenpaar erzeugt wird;
  - 55 Integrieren der gemessenen ersten Ströme über die Zeit, um eine erste Ladung zu erhalten;
  - 60 Integrieren der gemessenen zweiten Ströme über die Zeit, um eine zweite Ladung zu erhalten;
  - 65 Abziehen der zweiten Ladung von der ersten Ladung, um eine rauschverminderte Ladung zu erhalten; und
  - 70 Korrelieren der Konzentration des Analyten mit der rauschverminderten Ladung.
- 55 31. Verfahren nach Anspruch 24, wobei das Verfahren, vor den Stufen des Inkontaktbringens und Bestimmens, die weiteren Stufen umfaßt:

**EP 0 958 495 B1**

Bereitstellen des elektrochemischen Sensors nach irgendeinem der Ansprüche 1 bis 25, wobei der Sensor eines oder mehrere Paare von sich gegenüberliegenden Elektroden aufweist, wobei jedes Elektrodenpaar eine Arbeitselektrode, eine Gegenelektrode und eine Meßzone zwischen der Arbeitselektrode und der Gegenelektrode aufweist,

- 5        Messen einer Kapazitanz von wenigstens einem der Elektrodenpaare; und  
Errechnen des Volumens der Meßzone aus der Kapazitanzmessung.

32. Verfahren nach Anspruch 24, wobei der Sensor einen Redoxmediator auf der Arbeitselektrode aufweist, und wobei die molare Menge des Redoxmediators in einer reduzierten Form vor der Einführung der Probe geringer ist als, auf stöchiometrischer Basis, 5% der erwarteten molaren Menge des Analyten, der elektrolysiert werden soll, und wobei die Stufe der Bestimmung der Konzentration des Analyten umfaßt:

- 10      Elektrolysierten von weniger als etwa 1 µl der Probe.

- 15      33. Verfahren nach Anspruch 32, wobei der Sensor wenigstens zwei Arbeitselektroden aufweist, wobei jede Arbeitselektrode eine zugeordnete Meßzone aufweist, und wobei die Stufe der Bestimmung der Konzentration des Analyten das Mitteln von Messungen von den wenigstens zwei Arbeitselektroden umfaßt, und gegebenenfalls außerdem die Eliminierung von Messungen umfaßt, die einen Schwellenwert überschreiten, und gegebenenfalls außerdem das erneute Mitteln der Messungen ohne die eliminierten Messungen.

- 20      34. Ein Analytenmeßsystem, das umfaßt:

eine Probengewinnungseinrichtung, vorzugsweise ein Teil (54) zum Anstechen der Haut, wie beispielsweise eine Lanzette, um eine Patientenprobe zu erzeugen;

- 25      den elektrochemischen Sensor nach irgendeinem der Ansprüche 1 bis 23; und  
gegebenenfalls eine Transporteinrichtung, wie beispielsweise ein saugendes Material, eine Kapillarkammer, ein Sorbensmaterial oder eine Pumpe, um die Probe, die durch die Probengewinnungseinrichtung erzeugt wurde, in die Probenkammer oder die Meßzone zu transportieren.

- 30      35. System nach Anspruch 34, wobei die Einrichtung zum Anstechen der Haut ein Teil des Sensors ist.

36. Verfahren zur Messung eines Analyten in einer Patientenprobe, wobei das Verfahren umfaßt:

Inkontaktbringen des Patienten mit einem Analytenmeßsystem, wobei das System umfaßt:

- 35      eine Probengewinnungseinrichtung zur Erzeugung einer Patientenprobe; und  
den elektrochemischen Sensor nach irgendeinem der Ansprüche 1 bis 23, um den Analyten in der Probe zu messen,

- 40      Gewinnen einer Probe unter Verwendung der Probengewinnungseinrichtung;  
Transportieren eines Teils der Probe zu der Meßzone oder der Probenkammer des elektrochemischen Sensors, wobei die Stufe des Transportierens gegebenenfalls das Einsaugen der Probe in die Meßzone oder die Probenkammer unter Verwendung des Sorbensmaterials umfaßt; und  
Bestimmen der Konzentration des Analyten in der Probe durch Coulometrie.

- 45      37. Verfahren nach Anspruch 36, wobei die Probengewinnungseinrichtung ein Teil des Sensors ist.

38. Verfahren nach den Ansprüchen 36 oder 37, wobei die Probengewinnungseinrichtung ein Element zum Anstechen der Haut, wie beispielsweise eine Lanzette umfaßt, und der Schritt der Gewinnung einer Probe das Anstechen der Haut des Patienten an einem Ort, der nicht ein Finger des Patienten ist, umfaßt, um eine Probe zu erzeugen.

- 50      39. Verfahren zur Bestimmung einer Konzentration eines Analyten in einer Probe, wobei das Verfahren die Schritte umfaßt:

- 55      Verbinden der Elektroden eines elektrochemischen Sensors, der eine Arbeitselektrode, eine Gegenelektrode und eine Probenkammer aufweist, um die Probe in einem elektrolytischen Kontakt mit der Arbeitselektrode und der Gegenelektrode zu halten, mit der externen Elektronik einer Meßvorrichtung;  
Inkontaktbringen der Probe mit dem Sensor;

**EP 0 958 495 B1**

- Halten der Probe in einer strömungsfreien Weise innerhalb der Probenkammer;  
Anlegen eines Potentials zwischen der Arbeits- und der Gegenelektrode, um den Analyten in einem Teil der Probe innerhalb der Probenkammer zu elektrolyseren, wobei der Teil der Probe, in der der Analyt elektrolysiert wird, ein Volumen von weniger als 1 µl aufweist;
- 5 Messen des Stroms, der durch den elektrochemischen Sensor erzeugt wird, zu einer Vielzahl von Zeitpunkten, während der Analyt in dem Teil der Probe elektrolysiert wird; und  
Bestimmen, durch Coulometrie, einer Konzentration des Analyten in der Probe, unter Verwendung der gemessenen Ströme.
- 10 40. Sensor nach Anspruch 7, wobei der Sensor außerdem ein zweites Elektronenübertragungsmittel aufweist, wie beispielsweise ein Enzym, das auf dem Träger aufgetragen ist und mit dem Redoxmediator in Kontakt ist, wobei das zweite Elektronenübertragungsmittel gegebenenfalls auf dem Träger immobilisiert ist.
- 15 41. Verfahren zur Bestimmung einer Konzentration eines Analyten in einer Probe, das die Schritte umfaßt:
- Inkontaktbringen der Probe mit dem Sensor nach Anspruch 7 oder Anspruch 40, und  
Korrieren der Konzentration des Analyten in der Probe mit einer Veränderung des Oxidationszustands des Redoxmediators in Gegenwart von Analyten.
- 20 42. Verfahren nach Anspruch 41, wobei der Sensor einen optischen Sensor umfaßt, und die Stufe des Korrierens der Konzentration des Analyten umfaßt:
- Bestrahlen des Redoxmediators mit Licht;  
Messen der Reaktion des Redoxmediators auf die Bestrahlung mit Licht; und  
25 Korrieren der Konzentration des Analyten mit der gemessenen Antwort des Redoxmediators.
43. Verfahren nach Anspruch 42, wobei die Stufe der Messung der Antwort des Redoxmediators auf die Bestrahlung mit Licht das Messen der Absorption oder des Transmissionsgrads des eingestrahlten Lichts durch den Redoxmediator umfaßt.
- 30 44. Verfahren nach Anspruch 42, wobei der Schritt der Messung der Antwort des Redoxmediators auf Bestrahlung mit Licht das Messen der Fluoreszenz des Redoxmediators nach der Bestrahlung mit Licht, oder die Messung der Reflexion von Licht durch den Redoxmediator umfaßt.
45. Verfahren nach Anspruch 41, wobei der Sensor einen elektrochemischen Sensor umfaßt, und der Schritt der Korrelation der Konzentration des Analyten umfaßt:
- Anlegen eines elektrischen Potentials an den Redoxmediator;  
40 Messen eines Stroms in einem oder mehreren Intervallen, wobei der Strom als Reaktion auf die Elektrolyse des Redoxmediators in Gegenwart des Analyten erzeugt wird; und  
Korrieren der Konzentration des Analyten mit dem gemessenen Strom.
46. Verfahren nach Anspruch 41, wobei der Redoxmediator einen Übergangsmetallkomplex umfaßt, wie beispielsweise einen Osmiumkomplex, und vorzugsweise Osmium, das mit wenigstens einem Liganden mit einem stickstoffhaltigen Heterocyclus komplexiert ist, wie beispielsweise mit 2,2'-Bipyridin, 1,10-Phenanthrolin oder einem Derivat davon, vorzugsweise einem Mono-, Di- oder Polyalkoxyderivat von 2,2'-Bipyridin oder 1,10-Phenanthrolin, und noch stärker bevorzugt mit 4,4'-Dialkoxy-2,2'-bipyridin oder 4,7-Dialkoxy-1,10-phenanthrolin, wobei das Verhältnis von Kohlenstoff zu Sauerstoff der funktionalen Alkoxygruppen ausreicht, um die Löslichkeit des Übergangsmetallkomplexes in Wasser vor dem Vernetzen zu gewährleisten.
- 50 47. Verfahren nach Anspruch 46, wobei der stickstoffhaltige Heterocyclus 4,4'-Dimethoxy-2,2'-bipyridin oder 4,7-Dimethoxy-1,10-phenanthrolin umfaßt.
48. Verfahren nach Anspruch 46, wobei der Osmiumkomplex mit einem polymeren Liganden komplexiertes Osmium umfaßt, wobei der polymere Ligand einen stickstoffhaltigen Heterocyclus umfaßt.
- 55 49. Verfahren nach Anspruch 48, wobei das Polymer Poly(4-vinylpyridin) oder Poly(1-vinylimidazolin) umfaßt.

50. Verfahren nach Anspruch 49, wobei der Redoxmediator Os [4,4'-Dimethoxy-2,2'-bipyridin]<sub>2</sub>Cl<sup>+/+2</sup> oder Os[4,7-Dimethoxy-1,10-phenanthrolin]<sub>2</sub>Cl<sup>+/+2</sup> komplexiert mit Poly(1-vinylimidazol) umfaßt.
- 5 51. Sensor nach Anspruch 7, wobei ein Teil des luftoxidierbaren Redoxmediators oxidiert wird, wenn der analytische Sensor in einer Atmosphäre verpackt wird, die molekularen Sauerstoff enthält.
52. Verfahren nach Anspruch 50, wobei sich mehr als 90% des Redoxmediators nach einer Lagerung für mehr als einen Monat in einem oxidierten Zustand befinden.
- 10 53. Analytenmeßsystem, das umfaßt:
- a. einen Sensor nach einem der Ansprüche 1-23, 40 und 51; und
  - b. ein Coulometer, das funktionell mit dem Sensor verbunden ist und so ausgelegt ist, dass es die kumulative elektrische Ladung mißt, die durch den Sensor fließt.
- 15

#### Revendications

1. DéTECTEUR électrochimique pour déterminer la concentration d'un analyte dans un échantillon, le détecteur comprenant :
- 20 au moins une électrode de travail (22) ;  
au moins une électrode auxiliaire (24) ;  
lesquelles électrodes, en utilisation, sont raccordées à l'électronique externe d'un instrument de mesure ;  
25 au moins une chambre à échantillon (26), dans lequel ladite chambre à échantillon est :  
  
(i) une chambre à échantillon pour maintenir l'échantillon en contact électrolytique avec l'électrode de travail et dimensionnée pour contenir un maximum de 1 µl d'échantillon environ, ou  
(ii) une chambre à échantillon comprenant au moins une zone de mesure, dimensionnée pour contenir un maximum de 1 µl d'échantillon environ, dans laquelle la zone de mesure est limitée sur au moins deux 30 côtés par l'électrode de travail et l'électrode auxiliaire ;  
  
ledit détecteur contenant un médiateur d'oxydoréduction non lixiviable sur l'électrode de travail ; et  
35 ledit détecteur contenant facultativement un sorbant (34) disposé au moins partiellement à l'intérieur de la chambre à échantillon ou au moins partiellement à l'intérieur de la zone de mesure.
2. DéTECTEUR selon la revendication 1, dans lequel l'électrode de travail et l'électrode auxiliaire sont composées de métal ou de carbone ; et le détecteur comprend le médiateur d'oxydoréduction non lixiviable sur l'électrode de travail.
- 40 3. DéTECTEUR selon la revendication 2, dans lequel le détecteur comprend en outre un second agent de transfert électronique, de préférence une enzyme telle que la glucose oxydase, sur l'électrode de travail, dans lequel le second agent de transfert est facultativement immobilisé sur l'électrode de travail et/ou est facultativement non lixiviable.
- 45 4. DéTECTEUR selon la revendication 1, dans lequel l'électrode de travail et l'électrode auxiliaire sont composées de métal ou de carbone, et le détecteur comprend un sorbant disposé au moins partiellement à l'intérieur de la chambre à échantillon ou au moins partiellement à l'intérieur de la zone de mesure.
- 50 5. DéTECTEUR selon l'une quelconque des revendications 1 à 4, dans lequel la chambre à échantillon, ou la zone de mesure, est dimensionnée pour contenir un maximum de 0,5 µl environ, de préférence un maximum de 0,2 µl environ, de préférence un maximum de 0,1 µl environ d'échantillon.
- 55 6. DéTECTEUR selon l'une quelconque des revendications 1 à 5, dans lequel le médiateur d'oxydoréduction est immobilisé sur l'électrode de travail.
7. DéTECTEUR selon l'une quelconque des revendications 1 à 6, dans lequel le médiateur d'oxydoréduction est un médiateur d'oxydoréduction oxydable à l'air, avec de préférence au moins 90 % du médiateur d'oxydoréduction

oxydable à l'air à l'état oxydé avant l'introduction de l'échantillon.

8. Détecteur selon l'une quelconque des revendications 1 à 7, dans lequel le médiateur d'oxydoréduction comprend un complexe métallique de transition, tel qu'un complexe d'osmium, de ruthénium, de fer ou de cobalt, et de préférence un complexe d'osmium avec au moins un ligand ayant un composé hétérocyclique azoté, tel que la bipyridine-2,2', le diméthyl-4,4'bipyridine-2,2', le dialkoxy-4,4'bipyridine-2,2', la phénanthroline-1,10, le diméthyl-4,7 phénanthroline-1,10, le dialkoxy-4,7 phénanthroline-1,10, ou les dérivés de ceux-ci.
9. Détecteur selon la revendication 8, dans lequel le ligand ayant un composé hétérocyclique azoté comprend de la bipyridine-2,2', de la phénanthroline-1,10, ou un dérivé de celles-ci, tel qu'un dérivé mono-, di- ou polyalkoxy de la bipyridine-2,2' ou de la phénanthroline-1,10, dans lequel le rapport carbone sur oxygène des groupements fonctionnels alkoxy est suffisant pour conserver la solubilité du complexe métallique de transition dans l'eau avant la réticulation.
10. Détecteur selon la revendication 8 ou 9, dans lequel le rapport carbone sur oxygène des groupements fonctionnels alkoxy est suffisant pour conserver la solubilité du complexe métallique de transition dans l'eau avant la réticulation.
11. Détecteur selon l'une quelconque des revendications 1 à 10, dans lequel le sorbant a un volume mort de 5 % à 50 % environ, de préférence de 10 % à 25 % environ du volume total du sorbant.
12. Détecteur selon l'une quelconque des revendications 1 à 11, dans lequel le détecteur comprend en outre une ou plusieurs électrodes de travail supplémentaires.
13. Détecteur selon l'une quelconque des revendications 1 à 12, dans lequel au moins une électrode de travail et au moins une électrode auxiliaire forment au moins une paire d'électrodes en regard, dans lequel facultativement chaque paire réagit à un analyte spécifique.
14. Détecteur selon la revendication 13, dans lequel la distance séparant l'électrode de travail de l'électrode auxiliaire n'excède pas 0,2 mm environ, ou 0,1 mm environ, ou 0,05 mm environ.
15. Détecteur selon la revendication 13, dans lequel au moins une paire d'électrodes en regard est composée d'une électrode de travail comprenant un médiateur d'oxydoréduction et une enzyme non lixiviables, et dans lequel au moins une autre paire d'électrodes en regard est composée d'une électrode de travail comprenant un médiateur d'oxydoréduction non lixiviable en l'absence de l'enzyme.
16. Détecteur selon la revendication 15, comprenant en outre une troisième paire d'électrodes (46) n'ayant ni médiateur d'oxydoréduction ni enzyme sur l'électrode de travail.
17. Détecteur selon l'une quelconque des revendications 1 à 16, dans lequel l'électrode de travail comprend un premier bras (122) et l'électrode auxiliaire comprend un second bras (124), une partie du premier bras chevauchant une partie du second bras, dans lequel la zone de mesure, ou la chambre à échantillon, comprend une région (21) entre les parties chevauchantes du premier et du second bras.
18. Détecteur selon la revendication 17, dans lequel le premier bras a une longueur supplémentaire et la partie chevauchante du premier bras a une largeur, dans lequel le rapport de la longueur supplémentaire du premier bras sur la largeur de la partie chevauchante du premier bras varie de 0,1/1.à 50/1, de préférence de 1/1 à 15/1, et de manière préférée entre toutes de 4/1 à 10/1.
19. Détecteur selon la revendication 18, dans lequel le premier et le second bras se coupent à un angle supérieur à 0 degré.
20. Détecteur selon l'une quelconque des revendications 1 à 19, dans lequel le sorbant comporte un matériau en poudre disposé sur l'électrode de travail.
21. Détecteur selon la revendication 13, dans lequel ladite paire d'électrodes en regard comprend un matériau de base (102) ayant une encoche (104) et au moins une de l'électrode de travail et de l'électrode auxiliaire disposée dans l'encoche.

22. Détecteur selon l'une quelconque des revendications 1 à 21, comprenant en outre un matériau de remplissage, de préférence un matériau de remplissage hydrophile, dans lequel le matériau de remplissage est disposé dans la zone de mesure ou dans la chambre à échantillon, pour réduire un volume de la zone de mesure ou de la chambre à échantillon disponible pour l'échantillon.
- 5 23. Détecteur selon l'une quelconque des revendications 1 à 22, dans lequel le détecteur produit un signal dans une solution tampon contenant 10 mM de glucose qui est au moins 9 fois plus fort qu'un signal produit dans une solution tampon sans glucose.
- 10 24. Procédé pour déterminer une concentration d'un analyte dans un échantillon, comportant la mise en contact de l'échantillon avec le détecteur électrochimique selon l'une quelconque des revendications 1 à 23, et la détermination de la concentration de l'analyte dans l'échantillon par coulométrie.
- 15 25. Procédé selon la revendication 24, dans lequel l'étape de mise en contact est réalisée en mettant en contact l'échantillon avec le sorbant pour introduire par effet de mèche l'échantillon dans la chambre à échantillon ou dans la zone de mesure.
26. Procédé selon la revendication 24, dans lequel la chambre à échantillon se remplit par capillarité.
- 20 27. Procédé selon la revendication 24, dans lequel l'étape de détermination de la concentration de l'analyte comporte les phases suivantes :
- 25      électrolyse d'eau au moins 90 % de l'analyte présent dans la zone de mesure par application d'un potentiel à travers l'électrode de travail et l'électrode auxiliaire, de préférence en moins de 5 minutes environ, et de manière préférée entre toutes en moins de 1 minute environ ;  
détermination d'une charge électrique utilisée pour électrolyser l'analyte ;  
et corrélation entre la charge électrique et la concentration de l'analyte dans l'échantillon ;  
dans lequel l'étape de détermination est facultativement réalisée selon les phases suivantes :
- 30      mesure d'un courant généré au niveau de l'électrode de travail à deux instants ou plus pendant l'électrolyse de l'analyte ;  
intégration dans le temps des courants mesurés pour obtenir la charge électrique utilisée pour électrolyser l'analyte.
- 35 28. Procédé selon la revendication 24, dans lequel l'étape de détermination de la concentration de l'analyte par coulométrie comporte les phases suivantes :
- 40      électrolyse d'une partie de l'analyte par application d'un potentiel à travers l'électrode de travail et l'électrode auxiliaire ;  
mesure d'un courant généré au niveau de l'électrode de travail à deux instants ou plus pendant l'électrolyse ;  
extrapolation d'une courbe de courant basée sur les courants mesurés ;  
intégration dans le temps de la courbe de courant pour obtenir une charge électrique nécessaire pour électrolyser au moins 90 % de l'analyte ;  
et corrélation entre la charge électrique et la concentration de l'analyte dans l'échantillon.
- 45 29. Procédé selon la revendication 24, dans lequel le détecteur électrochimique est composé d'une première et d'une seconde paire d'électrodes, chaque paire comportant une électrode de travail, dans lequel ladite première paire d'électrode comprend un médiateur d'oxydoréduction non lixiviable et une enzyme non lixiviable sur l'électrode de travail, et dans lequel ladite seconde paire d'électrode comprend un médiateur d'oxydoréduction non lixiviable en l'absence d'enzyme.
- 50 30. Procédé selon la revendication 29, dans lequel l'étape de détermination de la concentration de l'analyte comporte les phases suivantes :
- 55      mesure pratiquement simultanée, et à deux instants ou plus, d'un premier courant généré au niveau de la première paire d'électrodes et d'un second courant généré au niveau de la seconde paire d'électrodes ;  
intégration dans le temps des premiers courants mesurés pour obtenir une seconde charge ;  
soustraction de la seconde charge de la première charge pour obtenir une charge à bruit réduit ;

et corrélation entre la concentration de l'analyte et la charge à bruit réduit.

31. Procédé selon la revendication 24, le procédé comportant, avant les étapes de mise en contact et de détermination, les autres phases suivantes :

5 fourniture du détecteur électrochimique selon l'une quelconque des revendications 1 à 23, dans lequel le détecteur a une ou plusieurs paires d'électrodes en regard, chaque paire d'électrodes étant composée d'une électrode de travail, d'une électrode auxiliaire et d'une zone de mesure entre l'électrode de travail et l'électrode auxiliaire ;  
10 mesure d'une capacité d'au moins une des paires d'électrodes ;  
et calcul du volume de la zone de mesure à partir de la mesure de capacité.

32. Procédé selon la revendication 24, dans lequel le détecteur comprend un médiateur d'oxydoréduction sur l'électrode de travail, et la quantité molaire de médiateur d'oxydoréduction sous forme réduite avant l'introduction de l'échantillon est inférieure, sur une base stoechiométrique, à 5 % de la quantité molaire théorique de l'analyte à électrolyser ; et dans lequel l'étape de détermination de la concentration de l'analyte comporte :

20 électrolyse de moins d'1 µl d'échantillon.

33. Procédé selon la revendication 32, dans lequel le détecteur comprend au moins deux électrodes de travail, chaque électrode de travail ayant une zone de mesure associée, et dans lequel l'étape de détermination de la concentration de l'analyte comporte le calcul de la moyenne des mesures réalisées sur lesdites électrodes de travail, et facultativement comporte en outre l'élimination des mesures excédant une valeur-seuil, et facultativement comporte en outre le recalcul de la moyenne des mesures sans les mesures éliminées.

- 25 34. Dispositif de mesure d'analyte comprenant :

moyen d'acquisition d'échantillons, de préférence un membre pour inciser la peau (54), tel qu'une lancette, pour produire un échantillon d'un patient ;  
30 le détecteur électrochimique selon l'une quelconque des revendications 1 à 23 ;  
et facultativement un moyen de transport, tel un matériau à effet de mèche, une chambre capillaire, un sorbant ou une pompe, pour transporter l'échantillon produit par le moyen d'acquisition d'échantillons vers la chambre à échantillon ou vers la zone de mesure.

- 35 35. Dispositif selon la revendication 34, dans lequel le membre pour inciser la peau fait partie intégrante du détecteur.

36. Procédé pour mesurer l'analyte dans un échantillon de patient, le procédé comprenant :

40 mise en contact du patient avec le dispositif de mesure d'analyte, le dispositif comprenant :

un moyen d'acquisition d'échantillon pour produire un échantillon de patient ;  
et le détecteur électrochimique selon l'une quelconque des revendications 1 à 23, pour mesurer l'analyte dans l'échantillon ;  
45 acquisition d'un échantillon avec le moyen d'acquisition d'échantillon ;  
transport d'une partie de l'échantillon vers la zone de mesure ou la chambre à échantillon du détecteur électrochimique, dans lequel l'étape de transport comprend facultativement l'introduction par effet de mèche de l'échantillon dans la zone de mesure ou dans la chambre à échantillon à l'aide du sorbant ;  
et la détermination de la concentration de l'analyte dans l'échantillon par coulométrie.

- 50 37. Procédé selon la revendication 36, dans lequel le moyen d'acquisition d'échantillon fait partie intégrante du détecteur.

38. Procédé selon les revendications 36 et 37, dans lequel le moyen d'acquisition d'échantillon comprend un membre pour inciser la peau, tel une lancette, et l'étape d'acquisition d'échantillon comporte l'incision de la peau du patient à un endroit autre que le doigt pour produire un échantillon.

- 55 39. Procédé pour déterminer une concentration d'un analyte dans un échantillon, le procédé comportant les étapes suivantes :

- raccordement des électrodes d'un détecteur électrochimique composé d'une électrode de travail, d'une électrode auxiliaire, et d'une chambre à échantillon pour maintenir l'échantillon en contact électrolytique avec l'électrode de travail et l'électrode auxiliaire, à l'électronique externe d'un appareil de mesure ;  
mise en contact de l'échantillon et du détecteur ;  
5      maintien de l'échantillon à l'intérieur de la chambre à échantillon sans circulation ;  
application d'un potentiel entre l'électrode de travail et l'électrode auxiliaire pour électrolyser l'analyte dans une partie de l'échantillon à l'intérieur de la chambre à échantillon, dans laquelle la partie de l'échantillon dans lequel l'analyte est électrolysé a un volume inférieur à 1 µl ;  
10     mesure du courant généré par le détecteur électrochimique à plusieurs instants pendant que l'analyte dans la partie de l'échantillon est électrolysé ;  
et détermination par coulométrie d'une concentration de l'analyte dans l'échantillon à l'aide des courants mesurés.
- 15     40. Détecteur selon la revendication 7, dans lequel le détecteur comprend en outre un second agent de transfert électronique, tel qu'une enzyme, enduit sur le support et en contact avec le médiateur d'oxydoréduction, dans lequel le second agent de transfert électronique est facultativement immobilisé sur le support.
- 20     41. Procédé pour déterminer une concentration d'un analyte dans un échantillon, comportant les étapes suivantes :  
mise en contact de l'échantillon avec le détecteur selon la revendication 7 ou la revendication 40 ;  
et corrélation entre la concentration de l'analyte dans l'échantillon et un changement d'état d'oxydation du médiateur d'oxydoréduction en présence d'analyte.
- 25     42. Procédé selon la revendication 41, dans lequel le détecteur comprend un détecteur optique, et l'étape de corrélation de la concentration de l'analyte comporte :  
irradiation du médiateur d'oxydoréduction avec de la lumière ;  
mesure de la réponse du médiateur d'oxydoréduction à l'irradiation par la lumière ;  
et corrélation entre la concentration de l'analyte et la réponse mesurée du médiateur d'oxydoréduction.  
30     43. Procédé selon la revendication 42, dans lequel l'étape de mesure de la réponse du médiateur d'oxydoréduction à l'irradiation par la lumière comporte la mesure de l'absorption, ou la transmittance, de la lumière irradiée par le médiateur d'oxydoréduction.
- 35     44. Procédé selon la revendication 42, dans lequel l'étape de mesure de la réponse du médiateur d'oxydoréduction à l'irradiation par la lumière comporte la mesure de la fluorescence du médiateur d'oxydation- réduction après irradiation par la lumière, ou la mesure de la réflexion de la lumière par le médiateur d'oxydoréduction.  
40     45. Procédé selon la revendication 41, dans lequel le détecteur comprenant un détecteur électrochimique, et l'étape de corrélation de la concentration de l'analyte comporte :  
application d'un potentiel électrique à travers le médiateur d'oxydoréduction ;  
mesure d'un courant à un ou plusieurs intervalles, le courant étant généré en réponse à l'électrolyse du médiateur d'oxydoréduction en présence de l'analyte ;  
et corrélation entre la concentration de l'analyte et le courant mesuré.  
45     46. Procédé selon la revendication 41, dans lequel le médiateur d'oxydoréduction comprend un complexe métallique de transition, tel qu'un complexe d'osmium, et de préférence à complexe d'osmium avec au moins un ligand ayant un composé hétérocyclique azoté, tel que la bipyridine-2,2', la phénanthroline-1,10, ou un dérivé de celles-ci, de préférence un dérivé mono-, di- ou polyalkoxy de la bipyridine-2,2' ou de la phénanthroline-1,10, et de manière préférée entre toutes comprend du dialkoxy-4,4' bipyridine-2,2' ou du dialkoxy-4,7 phénanthroline-1,10, dans lequel le rapport carbone sur oxygène des groupements fonctionnels alkoxy est suffisant pour conserver la solubilité du complexe métallique de transition dans l'eau avant la réticulation.  
50     47. Procédé selon la revendication 46, dans lequel le composé hétérocyclique azoté comprend du diméthoxy-4,4' bipyridine-2,2' ou du diméthoxy-4,7 phénanthroline-1,10.  
48. Procédé selon la revendication 46, dans lequel le complexe d'osmium comprend de l'osmium en complexe avec

**EP 0 958 495 B1**

un ligand polymérique, dans lequel le ligand polymérique comprend un composé hétérocyclique azoté.

49. Procédé selon la revendication 48, dans lequel le polymère comprend du poly(vinyle pyridine-4) ou du poly(vinyle imidazole-1).
- 5 50. Procédé selon la revendication 49, dans lequel le médiateur d'oxydoréduction comprend de l'Os(diméthoxy-4,4'-bipyridine-2,2')<sub>2</sub>Cl<sup>+/+2</sup> ou de l'Os(diméthoxy-4,7 phénanthroline-1,10)<sub>2</sub>Cl<sup>+/+2</sup> en complexe avec du poly(vinyle imidazole-1).
- 10 51. DéTECTeur selon la revendication 7, dans lequel une partie du médiateur d'oxydoréduction oxydable à l'air est oxydée au moment de l'emballage du détecteur analytique dans une atmosphère contenant de l'oxygène moléculaire.
- 15 52. Procédé selon la revendication 50, dans lequel plus de 90 % du médiateur d'oxydoréduction est à l'état oxydé après une période de stockage supérieure à un mois.

53. Dispositif de mesure d'analyte comprenant :

- 20 un détecteur selon l'une quelconque des revendications 1 à 23, 40 et 51 ;  
et un coulombmètre fonctionnellement raccordé au détecteur et configuré pour mesurer la charge électrique cumulée circulant dans le détecteur.

25

30

35

40

45

50

55

FIG. 1


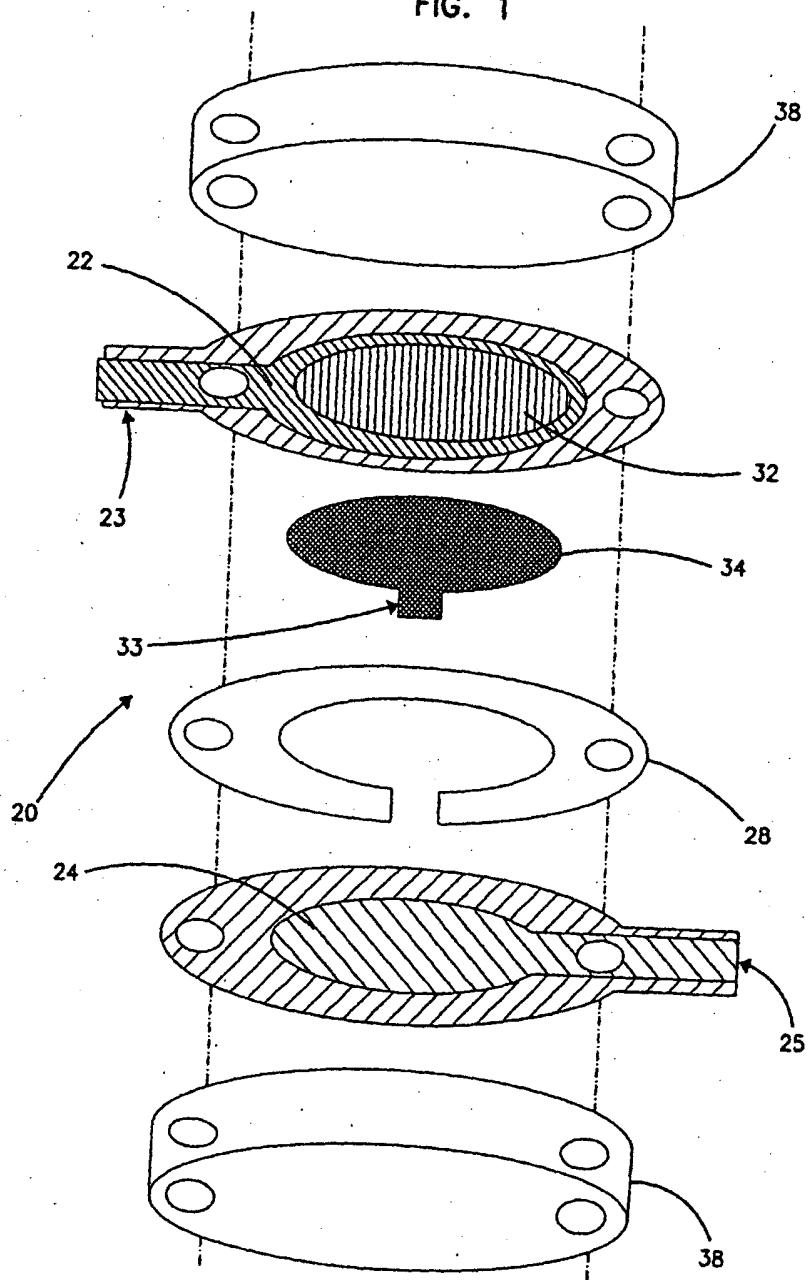


FIG. 2

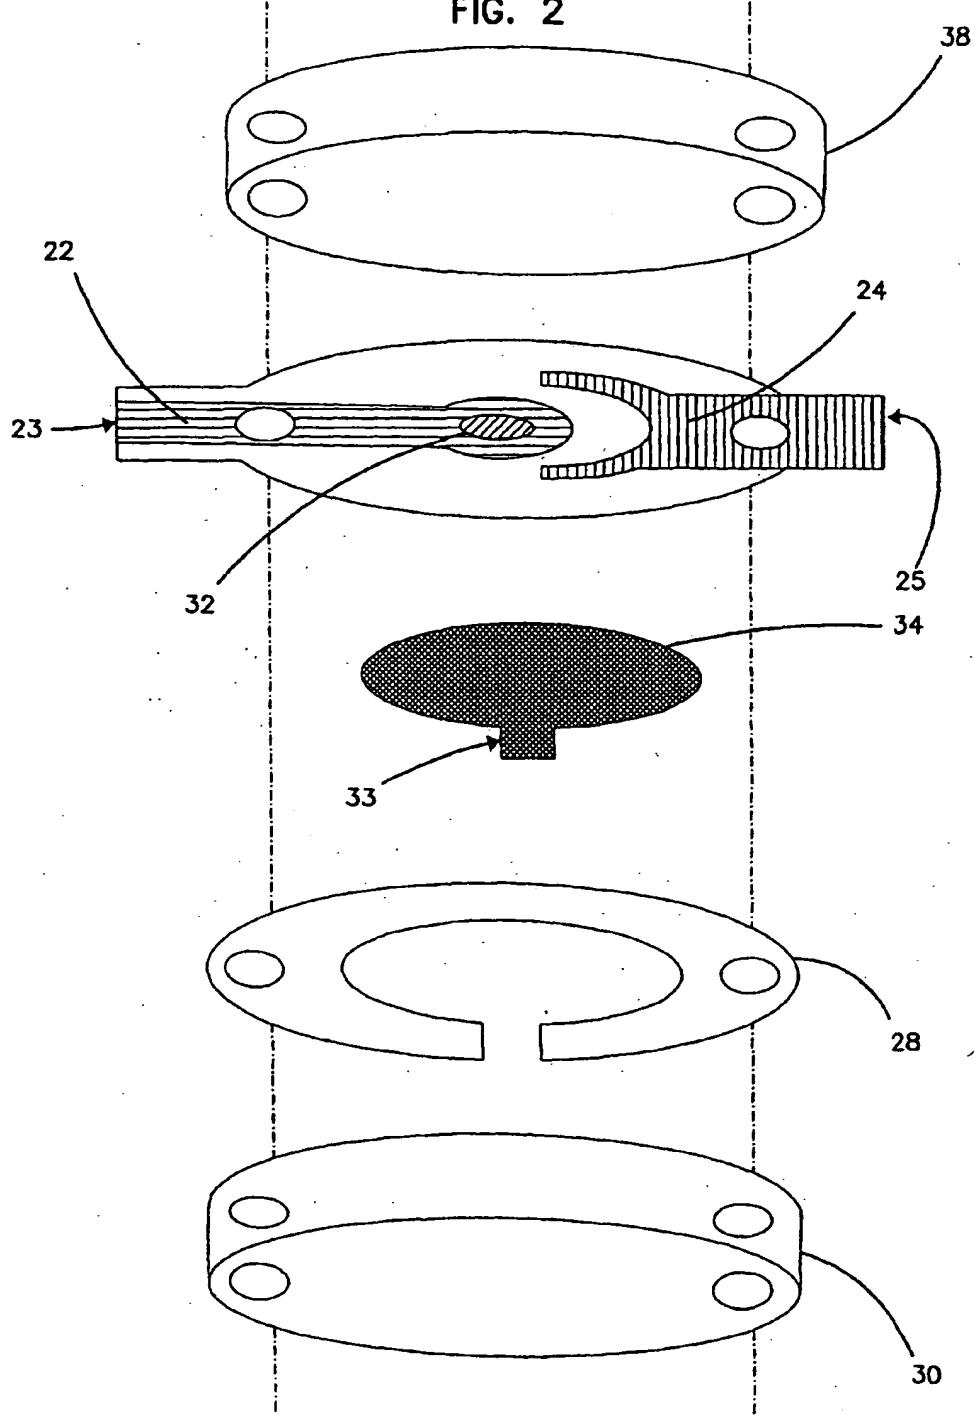

EP 0 958 495 B1

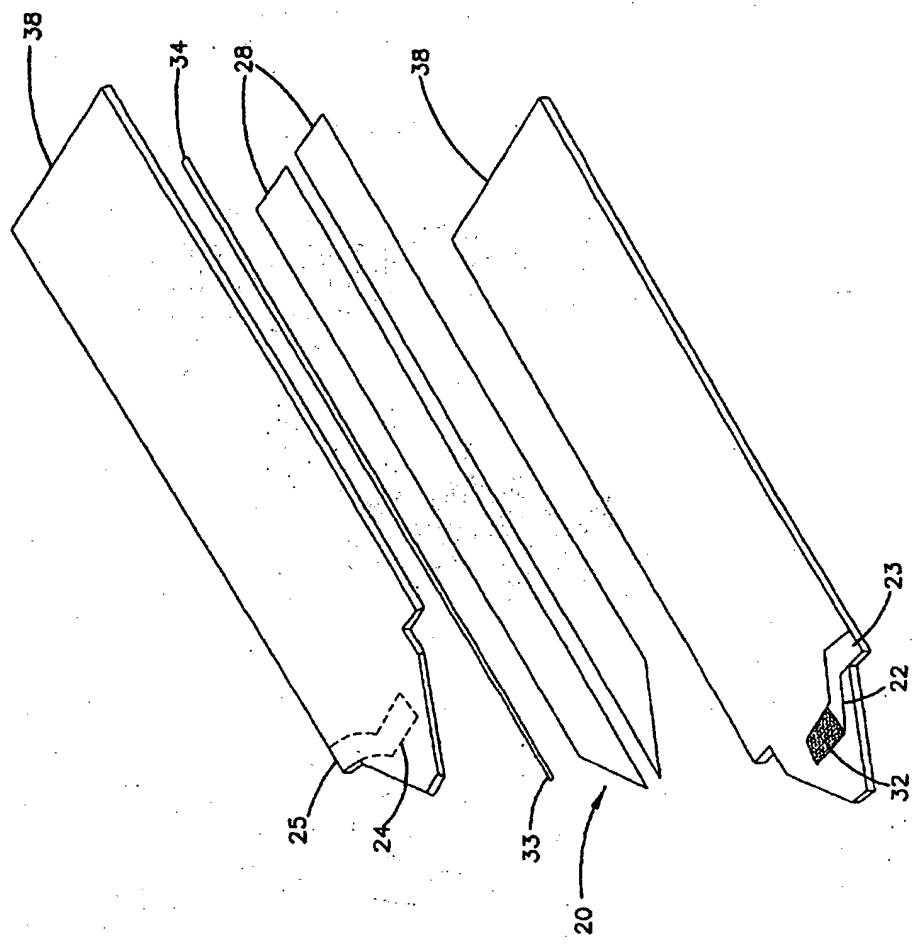


FIG. 3

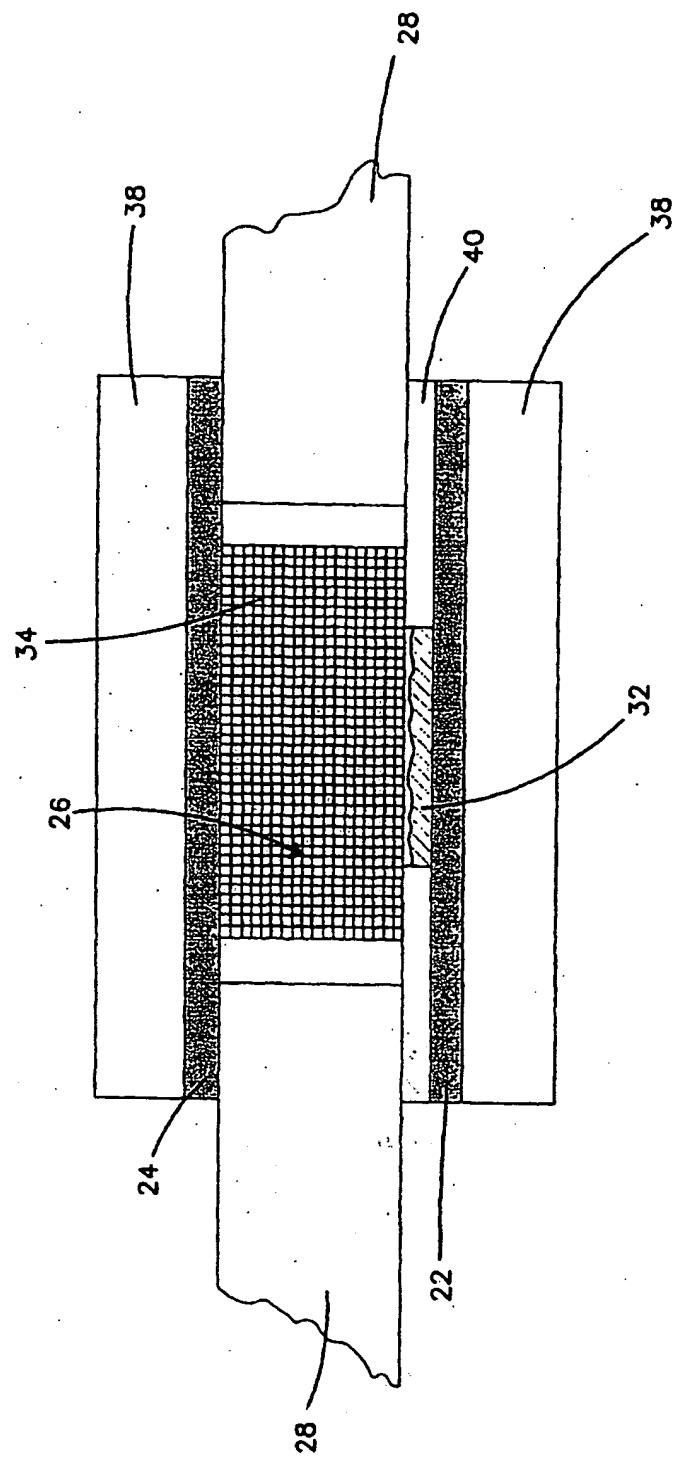
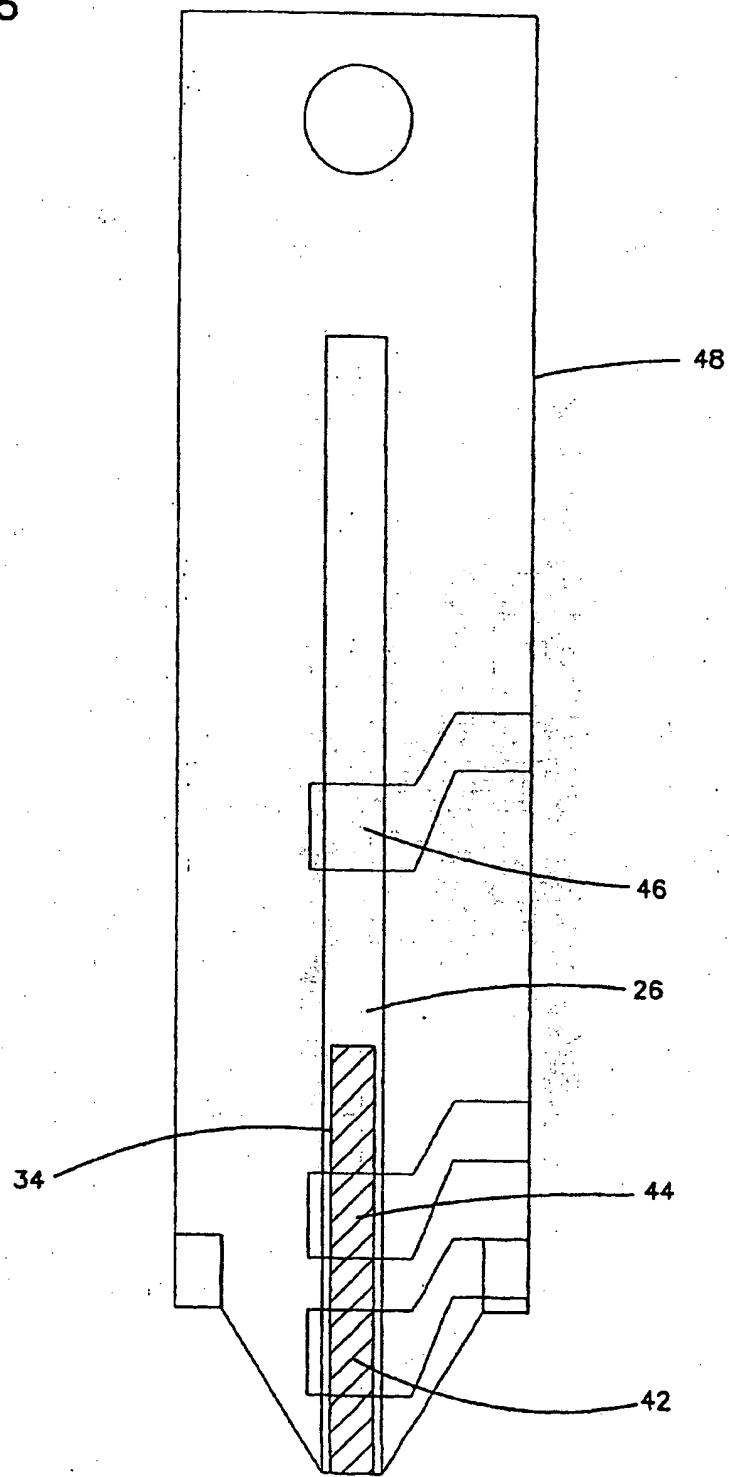


FIG. 4

FIG. 5



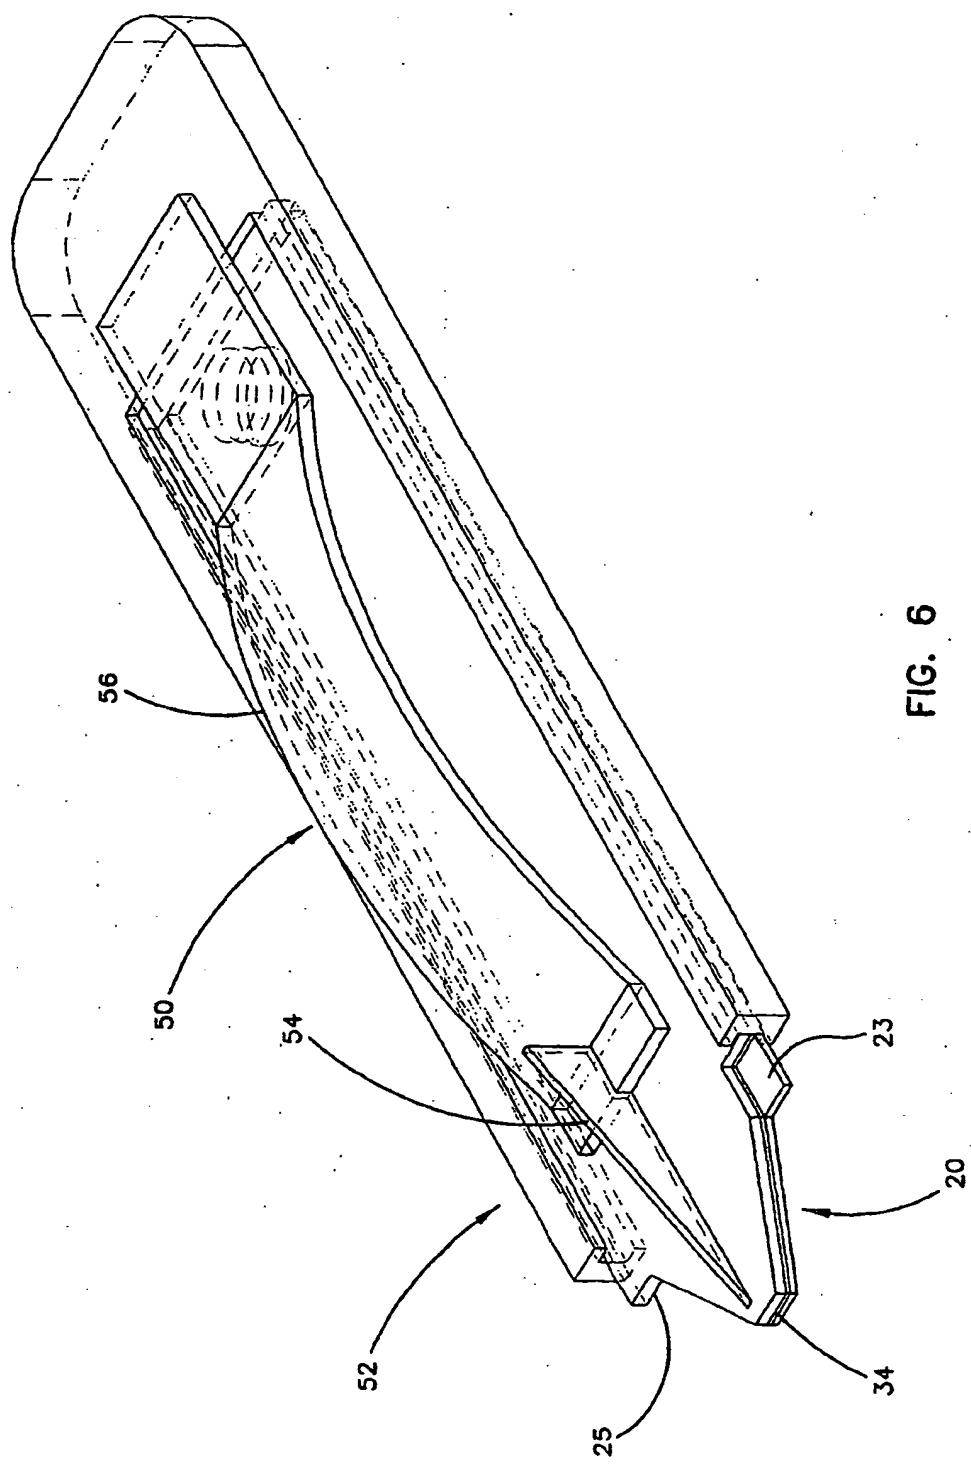


FIG. 6

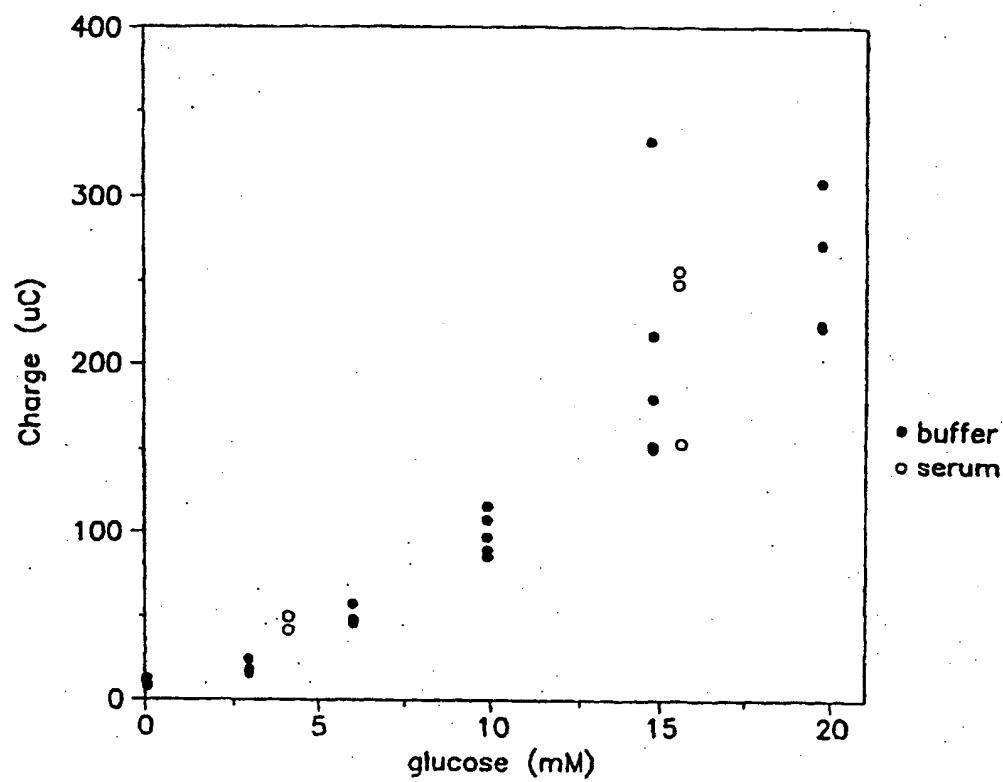


FIG. 7

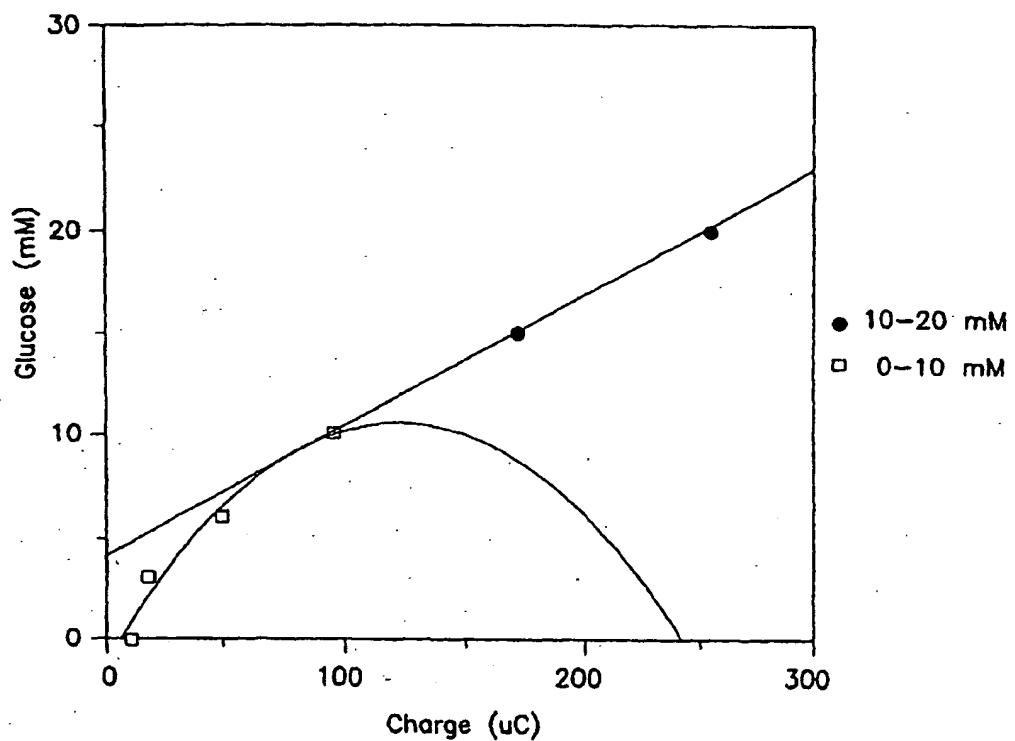


FIG. 8

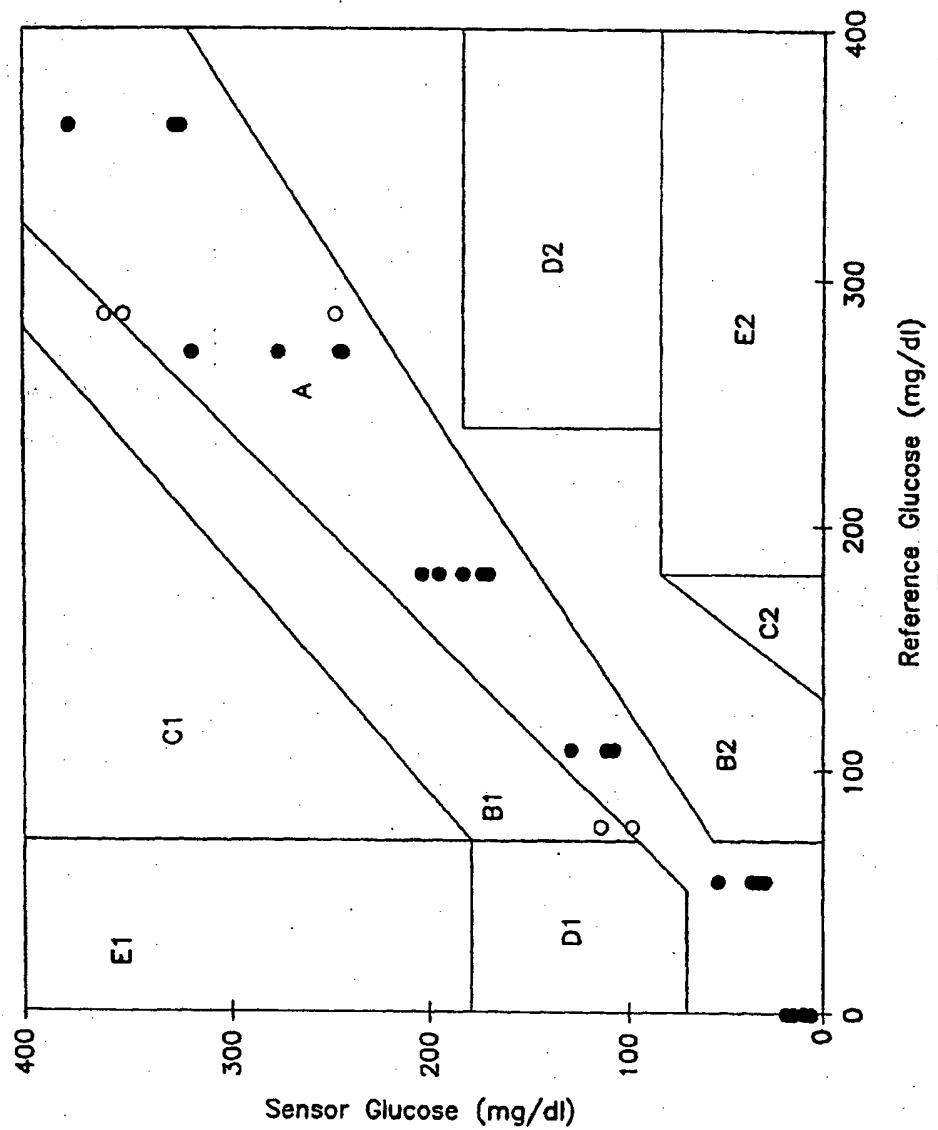


FIG. 9

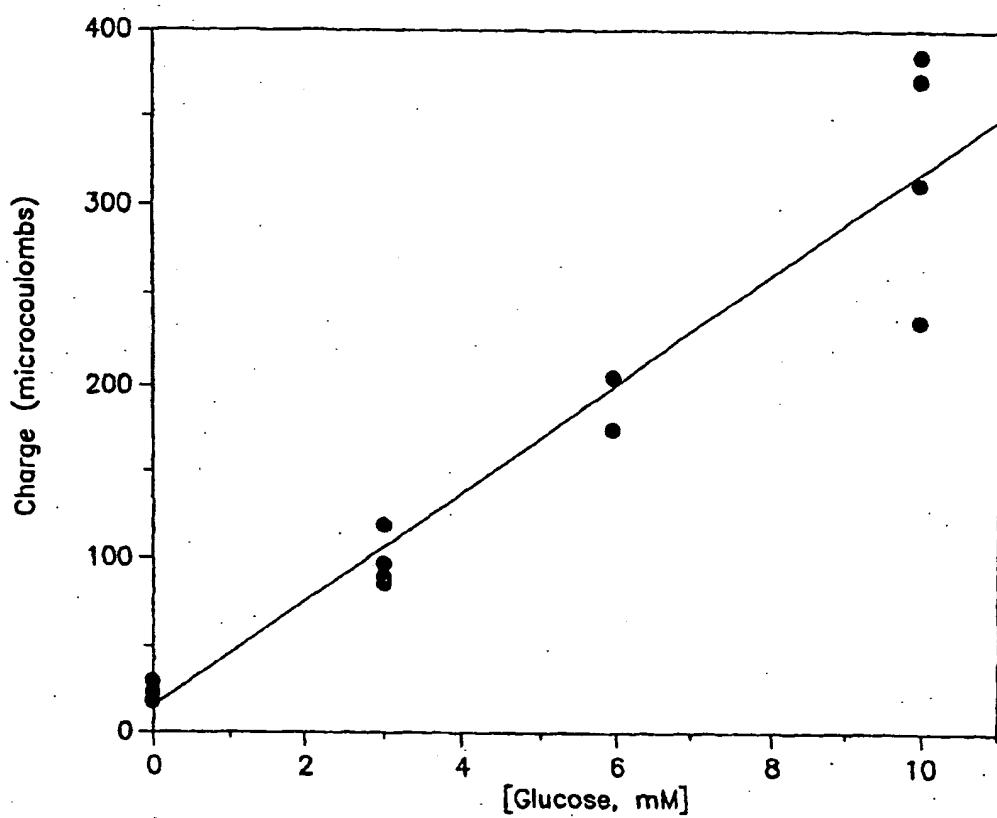


FIG. 10

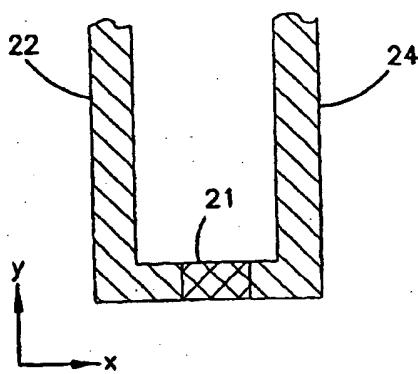


FIG. 11A

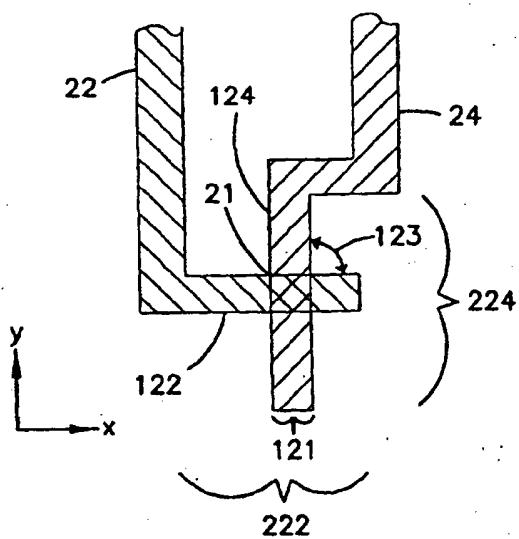


FIG. 11B

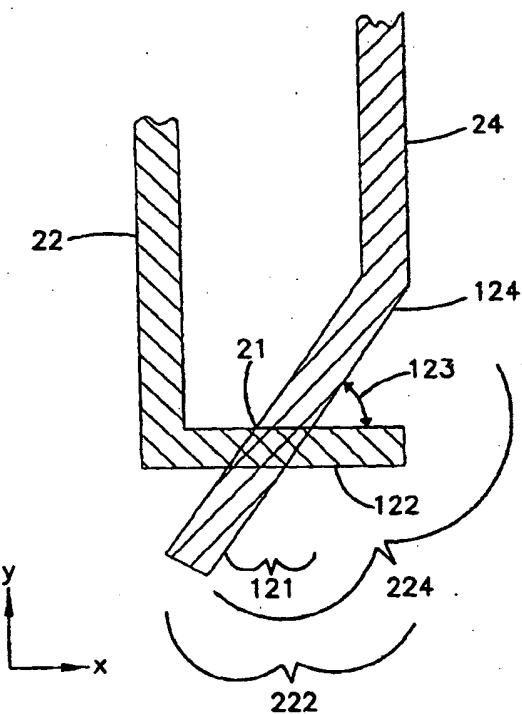


FIG. 11C

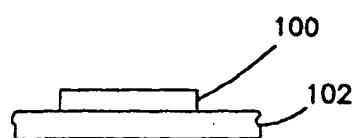


FIG. 12A

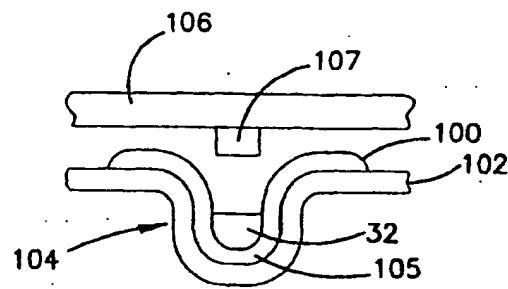


FIG. 12B



FIG. 13A

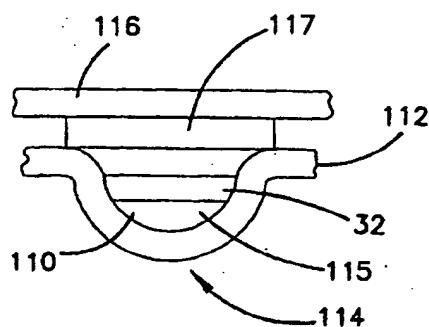


FIG. 13B

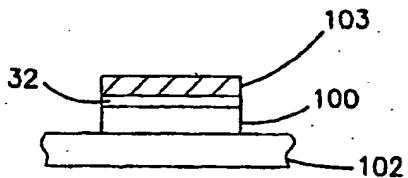


FIG. 14A

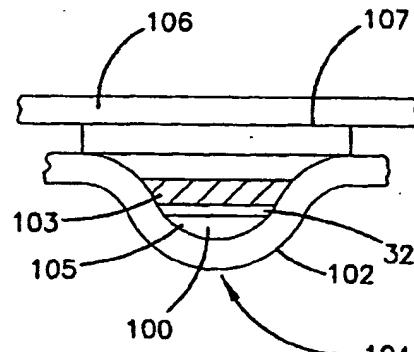


FIG. 14B

**THIS PAGE BLANK (USPTO)**